



SPC BENCHMARK 1™ FULL DISCLOSURE REPORT

**HUAWEI TECHNOLOGIES Co., LTD.
HUAWEI OCEANSTOR™ S8100 (4-NODE)**

SPC-1 V1.12

Submitted for Review: October 29, 2010

Submission Identifier: A00098

Revised: December 13, 2012

First Edition – October 2010

THE INFORMATION CONTAINED IN THIS DOCUMENT IS DISTRIBUTED ON AN AS IS BASIS WITHOUT ANY WARRANTY EITHER EXPRESS OR IMPLIED. The use of this information or the implementation of any of these techniques is the customer's responsibility and depends on the customer's ability to evaluate and integrate them into the customer's operational environment. While each item has been reviewed by Huawei Technologies Co., Ltd. for accuracy in a specific situation, there is no guarantee that the same or similar results will be obtained elsewhere. Customers attempting to adapt these techniques to their own environment do so at their own risk.

This publication was produced in the United States. Huawei Technologies Co., Ltd. may not offer the products, services, or features discussed in this document in other countries, and the information is subject to change with notice. Consult your local Huawei Technologies Co., Ltd. representative for information on products and services available in your area.

© Copyright Huawei Technologies Co., Ltd. 2010. All rights reserved.

Permission is hereby granted to reproduce this document in whole or in part, provided the copyright notice as printed above is set forth in full text on the title page of each item reproduced.

Trademarks

SPC Benchmark-1, SPC-1, SPC-1 IOPS, and SPC-1 LRT are trademarks of the Storage Performance Council. Huawei, the Huawei logo, and OceanStor are trademarks or registered trademarks of Huawei Technologies Co., Ltd. in the United States and other countries. All other brands, trademarks, and product names are the property of their respective owners.

Table of Contents

Audit Certification.....	vii
Audit Certification (<i>cont.</i>)	viii
Letter of Good Faith	ix
Executive Summary.....	10
Test Sponsor and Contact Information.....	10
Revision Information and Key Dates	10
Tested Storage Product (TSP) Description.....	10
Summary of Results	11
Storage Capacities, Relationships, and Utilization	11
Response Time – Throughput Curve	13
Response Time – Throughput Data.....	13
Priced Storage Configuration Pricing	14
Differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration.....	14
Priced Storage Configuration Diagram.....	15
Priced Storage Configuration Components.....	16
Configuration Information	17
Benchmark Configuration (BC)/Tested Storage Configuration (TSC) Diagram.	17
Storage Network Configuration	17
Host System and Tested Storage Configuration (TSC) Table of Components....	17
Benchmark Configuration/Tested Storage Configuration Diagram.....	18
Host System(s) and Tested Storage Configuration Components.....	19
Customer Tunable Parameters and Options	19
Tested Storage Configuration (TSC) Description	20
SPC-1 Workload Generator Storage Configuration	20
SPC-1 Data Repository.....	21
Storage Capacities and Relationships	21
SPC-1 Storage Capacities	21
SPC-1 Storage Hierarchy Ratios	21
SPC-1 Storage Capacities and Relationships Illustration	22
Logical Volume Capacity and ASU Mapping	22
Storage Capacity Utilization	23
SPC-1 Benchmark Execution Results.....	24
SPC-1 Tests, Test Phases, and Test Runs.....	24
Primary Metrics Test – Sustainability Test Phase	25

SPC-1 Workload Generator Input Parameters	25
Sustainability Test Results File	25
Sustainability – Data Rate Distribution Data (<i>MB/second</i>)	26
Sustainability – Data Rate Distribution Graph	27
Sustainability – I/O Request Throughput Distribution Data	28
Sustainability – I/O Request Throughput Distribution Graph	29
Sustainability – Average Response Time (ms) Distribution Data	30
Sustainability – Average Response Time (ms) Distribution Graph	31
Sustainability – Response Time Frequency Distribution Data	32
Sustainability – Response Time Frequency Distribution Graph	32
Sustainability – Measured Intensity Multiplier and Coefficient of Variation.....	33
Primary Metrics Test – IOPS Test Phase.....	34
SPC-1 Workload Generator Input Parameters	34
IOPS Test Results File.....	34
IOPS Test Run – I/O Request Throughput Distribution Data	35
IOPS Test Run – I/O Request Throughput Distribution Graph.....	35
IOPS Test Run – Average Response Time (ms) Distribution Data	36
IOPS Test Run – Average Response Time (ms) Distribution Graph	36
IOPS Test Run – Response Time Frequency Distribution Data	37
IOPS Test Run –Response Time Frequency Distribution Graph.....	37
IOPS Test Run – I/O Request Information	38
IOPS Test Run – Measured Intensity Multiplier and Coefficient of Variation	38
Primary Metrics Test – Response Time Ramp Test Phase	39
SPC-1 Workload Generator Input Parameters	39
Response Time Ramp Test Results File.....	39
Response Time Ramp Distribution (IOPS) Data.....	40
Response Time Ramp Distribution (IOPS) Graph	41
SPC-1 LRT™ Average Response Time (ms) Distribution Data.....	42
SPC-1 LRT™ Average Response Time (ms) Distribution Graph	42
SPC-1 LRT™ (10%) – Measured Intensity Multiplier and Coefficient of Variation	43
Repeatability Test	44
SPC-1 Workload Generator Input Parameters	44
Repeatability Test Results File	45
Repeatability 1 LRT – I/O Request Throughput Distribution Data.....	46
Repeatability 1 LRT – I/O Request Throughput Distribution Graph	46
Repeatability 1 LRT –Average Response Time (ms) Distribution Data	47
Repeatability 1 LRT –Average Response Time (ms) Distribution Graph	47
Repeatability 1 IOPS – I/O Request Throughput Distribution Data	48
Repeatability 1 IOPS – I/O Request Throughput Distribution Graph.....	48

Repeatability 1 IOPS –Average Response Time (ms) Distribution Data	49
Repeatability 1 IOPS –Average Response Time (ms) Distribution Graph	49
Repeatability 2 LRT – I/O Request Throughput Distribution Data.....	50
Repeatability 2 LRT – I/O Request Throughput Distribution Graph	50
Repeatability 2 LRT –Average Response Time (ms) Distribution Data	51
Repeatability 2 LRT –Average Response Time (ms) Distribution Graph.....	51
Repeatability 2 IOPS – I/O Request Throughput Distribution Data	52
Repeatability 2 IOPS – I/O Request Throughput Distribution Graph.....	52
Repeatability 2 IOPS –Average Response Time (ms) Distribution Data.....	53
Repeatability 2 IOPS –Average Response Time (ms) Distribution Graph	53
Repeatability 1 (LRT) Measured Intensity Multiplier and Coefficient of Variation	54
Repeatability 1 (IOPS) Measured Intensity Multiplier and Coefficient of Variation	54
Repeatability 2 (LRT) Measured Intensity Multiplier and Coefficient of Variation	54
Repeatability 2 (IOPS) Measured Intensity Multiplier and Coefficient of Variation	55
Data Persistence Test.....	56
SPC-1 Workload Generator Input Parameters	56
Data Persistence Test Results File	56
Data Persistence Test Results.....	57
Priced Storage Configuration Availability Date.....	58
Pricing Information.....	58
Tested Storage Configuration (TSC) and Priced Storage Configuration Differences.....	58
Anomalies or Irregularities	58
Appendix A: SPC-1 Glossary	59
“Decimal” (<i>powers of ten</i>) Measurement Units	59
“Binary” (<i>powers of two</i>) Measurement Units.....	59
SPC-1 Data Repository Definitions.....	59
SPC-1 Data Protection Levels	60
SPC-1 Test Execution Definitions	60
I/O Completion Types	62
SPC-1 Test Run Components	62
Appendix B: Customer Tunable Parameters and Options.....	63
Windows 2003 Server.....	63
S8100.....	63
Appendix C: Tested Storage Configuration (TSC) Creation	64
1. Configure the HBAs.....	64
2. Create RAID groups and LUNs in the data controller groups	64

raid_lun.script	64
3. Create disk groups and volumes	65
www_luns.script	66
www_elements.script	66
disk_volume.script	66
4. Create Windows stripe volumes	68
doSPC.bat	68
convertGPT.script	68
convertDynamic.script	69
createVolumes.script.....	70
Appendix D: SPC-1 Workload Generator Storage Commands and Parameters	72
Persistence Test Run 1 (write phase)	72
Persistence Test Run 2 (read phase)	73
Appendix E: SPC-1 Workload Generator Input Parameters	74
Primary Metrics Test, Repeatability Test, and Persistence Test Run 1	74
Persistence Test Run 2.....	74

AUDIT CERTIFICATION



Gradient
SYSTEMS

Michael Ko
 Huawei Symantec Technologies Co., Ltd.
 20245 Stevens Creek Blvd.
 Cupertino, CA 95014

October 29, 2010

The SPC Benchmark 1™ results listed below for the Huawei Symantec Oceanspace™ S8100 (*4-node*) were produced in compliance with the SPC Benchmark 1™ 1.12 Remote Audit requirements.

SPC Benchmark 1™ 1.12 Results	
Tested Storage Configuration (TSC) Name:	
Huawei Symantec Oceanspace™ S8100 (<i>4-node</i>)	
Metric	Reported Result
SPC-1 IOPS™	160,057.09
SPC-1 Price-Performance	CNY 49.03/SPC-1 IOPS™
Total ASU Capacity	92,180.000 GB
Data Protection Level	Protected (<i>Mirroring</i>)
Total TSC Price (including three-year maintenance)	CNY 7,847,296

The following SPC Benchmark 1™ Remote Audit requirements were reviewed and found compliant with 1.12 of the SPC Benchmark 1™ specification:

- A Letter of Good Faith, signed by a senior executive.
- The following Data Repository storage items, based on information supplied by Huawei Symantec Technologies Co., Ltd.:
 - ✓ Physical Storage Capacity and requirements.
 - ✓ Configured Storage Capacity and requirements.
 - ✓ Addressable Storage Capacity and requirements.
 - ✓ Capacity of each Logical Volume and requirements.
 - ✓ Capacity of each Application Storage Unit (ASU) and requirements.
- An appropriate diagram of the Benchmark Configuration (BC)/Tested Storage Configuration (TSC).
- Listings and commands to configure the Benchmark Configuration/Tested Storage Configuration, including customer tunable parameters that were changed from default values.

Storage Performance Council
 643 Bair Island Road, Suite 103
 Redwood City, CA 94062
AuditService@storageperformance.org
 650.556.9384

AUDIT CERTIFICATION (CONT.)

Huawei Symantec Oceanspace™ S8100 (4-node)
SPC-1 Audit Certification

Page 2

- SPC-1 Workload Generator commands and parameters used for the audited SPC Test Runs.
- The following Host System requirements, based on information supplied by Huawei Symantec Technologies Co., Ltd.:
 - ✓ The type of Host System including the number of processors and main memory.
 - ✓ The presence and version number of the SPC-1 Workload Generator on each Host System.
 - ✓ The TSC boundary within each Host System.
- The Test Results Files and resultant Summary Results Files received from Huawei Symantec Technologies Co., Ltd. for each of following were authentic, accurate, and compliant with all of the requirements and constraints of Clauses 4 and 5 of the SPC-1 Benchmark Specification:
 - ✓ Data Persistence Test
 - ✓ Sustainability Test Phase
 - ✓ IOPS Test Phase
 - ✓ Response Time Ramp Test Phase
 - ✓ Repeatability Test
- There were no differences between the Tested Storage Configuration (TSC) used for the benchmark and Priced Storage.
- The submitted pricing information met all of the requirements and constraints of Clause 8 of the SPC-1 Benchmark Specification.
- The Full Disclosure Report (FDR) met all of the requirements in Clause 9 of the SPC-1 Benchmark Specification.
- This successfully audited SPC measurement is not subject to an SPC Confidential Review.

Audit Notes:

There were no audit notes or exceptions.

Respectfully,

Walter E. Baker
SPC Auditor

Storage Performance Council
643 Bair Island Road, Suite 103
Redwood City, CA 94062
AuditService@storageperformance.org
650.556.9384

LETTER OF GOOD FAITH



©Huawei Symantec Technologies Co., Ltd.

Tiancheng Road 88#

Chengdu city

Sichuan province

China

Tel: 86-400-888-2333 Fax: 86-28-87897555

<http://www.huaweisymantec.com/en/>

Date: October 21, 2010

From: Huawei Symantec Technologies Co., Ltd.

To: Walter E. Baker, SPC Auditor
Gradient Systems, Inc.
643 Bair Island Road, Suite 103
Redwood City, CA 94063

Subject: SPC-1 Letter of Good Faith for the Huawei Symantec Oceanspace S8100 4-node

Huawei Symantec Technologies Co., Ltd. is the SPC-1 Test Sponsor for the above listed product. To the best of our knowledge and belief, the required SPC-1 benchmark results and materials we have submitted for that product are complete, accurate, and in full compliance with V1.12 of the SPC-1 benchmark specification.

In addition, we have reported any items in the Benchmark Configuration and execution of the benchmark that affected the reported results even if the items are not explicitly required to be disclosed by the SPC-1 benchmark specification.

Signed:

Su Liqing
Senior Vice President R&D

Date:

EXECUTIVE SUMMARY

Test Sponsor and Contact Information

Test Sponsor and Contact Information	
Test Sponsor Primary Contact	Huawei Technologies Co., Ltd. – http://www.huawei.com/en/ Eric He – eric.heji@huawei.com No. 1899, Xiyuan Road Chengdu, 611731 P.R. China Phone: 0086 28 65281999 FAX: 0086 28 64686419
Test Sponsor Alternate Contact	Huawei Technologies Co., Ltd. – http://www.huawei.com/en/ Xu Zhong – xuzhong@huawei.com No. 1899, Xiyuan Road Chengdu, 611731 P.R. China Phone: 0086 65281927 FAX: 0086 28 64696419
Auditor	Storage Performance Council – http://www.storageperformance.org Walter E. Baker – AuditService@StoragePerformance.org 643 Bair Island Road, Suite 103 Redwood City, CA 94063 Phone: (650) 556-9384 FAX: (650) 556-9385

Revision Information and Key Dates

Revision Information and Key Dates	
SPC-1 Specification revision number	V1.12
SPC-1 Workload Generator revision number	V2.1.0
Date Results were first used publicly	October 29, 2010
Date the FDR was submitted to the SPC	October 29, 2010
Date revised FDR was submitted to the SPC Updated company name, logo and product name to reflect the complete acquisition of Huawei Symantec by Huawei Technologies Co., Ltd.	December 13, 2012
Date the priced storage configuration is available for shipment to customers	currently available
Date the TSC completed audit certification	October 28, 2010

Tested Storage Product (TSP) Description

Huawei OceanStor™ S8100 storage system (hereinafter referred to as the S8100) is a new generation, high-end, storage product that is used by enterprises for mission-critical applications. Boasting high reliability, high performance, high scalability, large capacity, comprehensive data protection, and diversified value-added features, the S8100 is applicable to the scenarios of large-scaled core database, high availability computing, high performance computing, and integrated storage, backup, and retrieving of mass data, and is the best choice for investment saving.

Summary of Results

SPC-1 Results	
Tested Storage Product (TSP) Name: Huawei OceanStor™ S8100 (4-node)	
Metric	Reported Result
SPC-1 IOPS™	160,057.09
SPC-1 Price-Performance	CNY 49.03/SPC-1 IOPS™
Total ASU Capacity	92,160.000 GB
Data Protection Level	Protected (<i>Mirroring</i>)
Total TSP Price (including three-year maintenance)	CNY 7,847,296


SPC-1 IOPS™ represents the maximum I/O Request Throughput at the 100% load point.

Total ASU (Application Storage Unit) Capacity represents the total storage capacity read and written in the course of executing the SPC-1 benchmark.

A Data Protection Level of Protected using *Mirroring* configures two or more identical copies of user data.

Storage Capacities, Relationships, and Utilization

The following diagram and table document the various storage capacities, used in this benchmark, and their relationships, as well as the storage utilization values required to be reported.

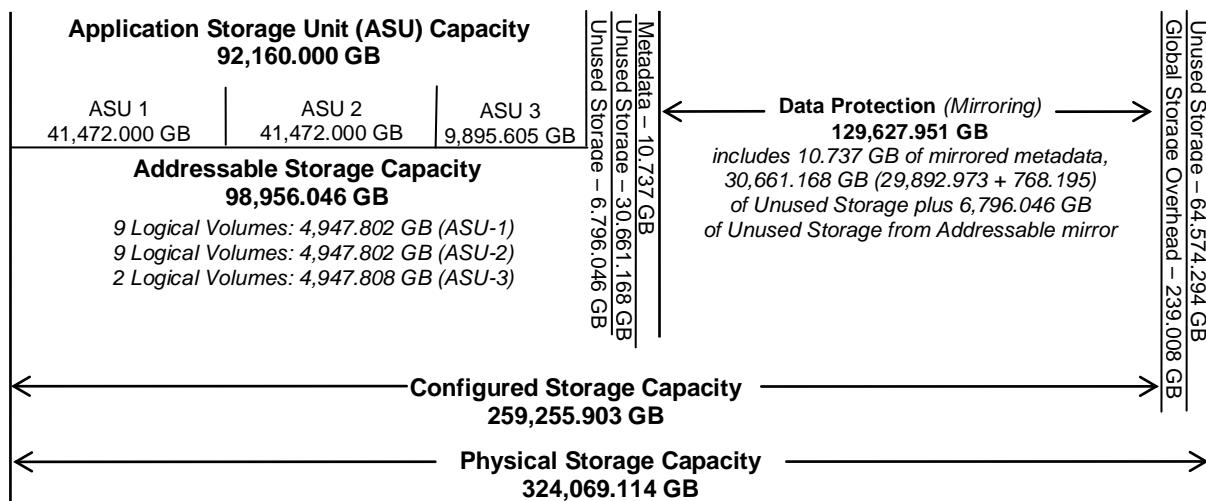

SPC-1 Storage Capacity Utilization	
Application Utilization	28.44%
Protected Application Utilization	56.88%
Unused Storage Ratio	43.04%

Application Utilization: Total ASU Capacity (*92,160.000 GB*) divided by Physical Storage Capacity (*324,069.114 GB*)

Protected Application Utilization: (Total ASU Capacity (*92,160.000 GB*) plus total Data Protection Capacity (*129,627.951 GB*) minus unused Data Protection Capacity (*37,457.214 GB*) divided by Physical Storage Capacity (*324,069.114 GB*)


Unused Storage Ratio: Total Unused Capacity (*139,488.632 GB*) divided by Physical Storage Capacity (*324,069.114 GB*) and may not exceed 45%.

Detailed information for the various storage capacities and utilizations is available on pages 21-22 in the Full Disclosure Report.

Response Time – Throughput Curve

The Response Time-Throughput Curve illustrates the Average Response Time (milliseconds) and I/O Request Throughput at 100%, 95%, 90%, 80%, 50%, and 10% of the workload level used to generate the SPC-1 IOPSTM metric.

The Average Response Time measured at any of the above load points cannot exceed 30 milliseconds or the benchmark measurement is invalid.

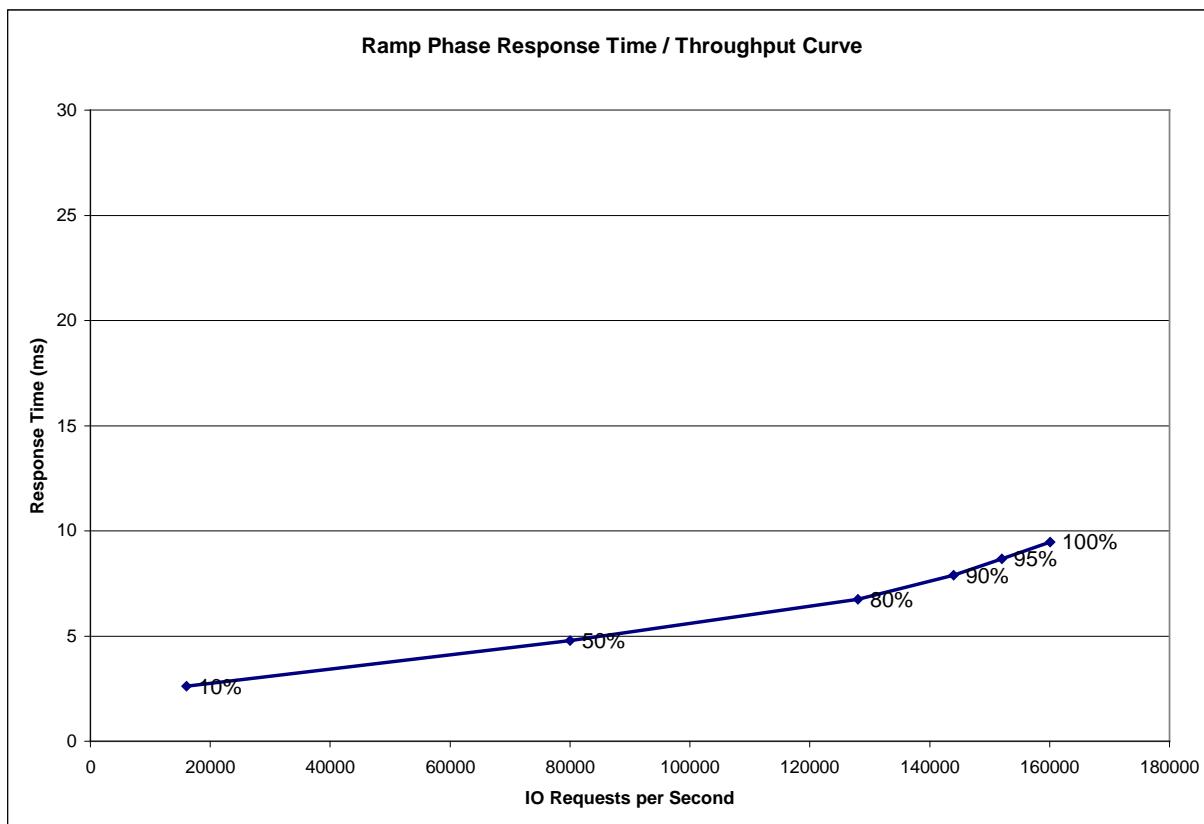

Response Time – Throughput Data

	10% Load	50% Load	80% Load	90% Load	95% Load	100% Load
I/O Request Throughput	16,006.65	80,015.25	128,000.15	144,016.01	152,005.22	160,057.09
Average Response Time (ms):						
All ASUs	2.62	4.79	6.74	7.90	8.68	9.47
ASU-1	3.34	6.00	8.49	9.98	10.98	12.03
ASU-2	3.11	5.98	9.11	11.07	12.44	13.85
ASU-3	0.86	1.68	2.00	2.10	2.14	2.12
Reads	5.42	9.66	14.19	16.99	18.89	20.93
Writes	0.80	1.61	1.89	1.98	2.02	2.01

Priced Storage Configuration Pricing

Product Name	Quantity	Unit Price(CNY)	Total Price(CNY)
S8100 System Rack	1	58,005	58,005
S8100 Service Controller Group *16 GB of memory, 8 GB per controller *8 - 4 Gbps SFPs	2	121,911	243,822
S8100 Management Switch Module	2	8,550	17,100
Fibre Channel 4-Port Adapter(4Gbps)	8	20,700	165,600
Ethernet 4-Port Adapter(1Gbps)	4	4,500	18,000
S8100 Expansion Rack	4	48,840	195,360
S8100 Data Controller Group (32GB) *32 GB of memory, 8 GB per controller *20 - 4 Gbps SFPs	4	90,504	362,018
S8100 Disk Expansion *4 - 4 Gbps SFPs	28	21,129	591,625
450GB/15Krpm (4Gbps) FC disk drive	144	7,950	1,144,800
600GB/15Krpm (4Gbps) FC disk drive	432	10,350	4,471,200
Storage Management Base License	1	33,000	33,000
Storage Management 1TB (>251TB)	324	600	194,400
UltraPath Base License	1	7,500	7,500
UltraPath For Windows/Linux License	2	750	1,500
S8000 First Installation Service , per Set per Time	1	249,691	249,691
UltraPath First Installation Service , per Set per Time	2	1,200	2,400
5-Meter Fiber Optic Cable	80	90	7,200
Blank panel	192	70	13,440
Dual-port Qlogic QLE2562 Fiber Channel HBA	4	17,659	70,636
Total (3-Year Maintenance Included)			7,847,296


The above pricing includes hardware maintenance and software support for a minimum of three years, 7 days per week, 24 hours per day. The hardware maintenance and software support provides the following:

- Acknowledgement of new and existing problems with four (4) hours.
- Onsite present of a qualified maintenance engineer or provision of a customer replaceable part within four (4) hours of the above acknowledgement for any hardware failure that results in an inoperative Price Storage Configuration that can be remedied by the repair or replacement of a Priced Storage Configuration component.

Differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration

There were no differences between the TSC and Priced Storage Configuration.

Priced Storage Configuration Diagram

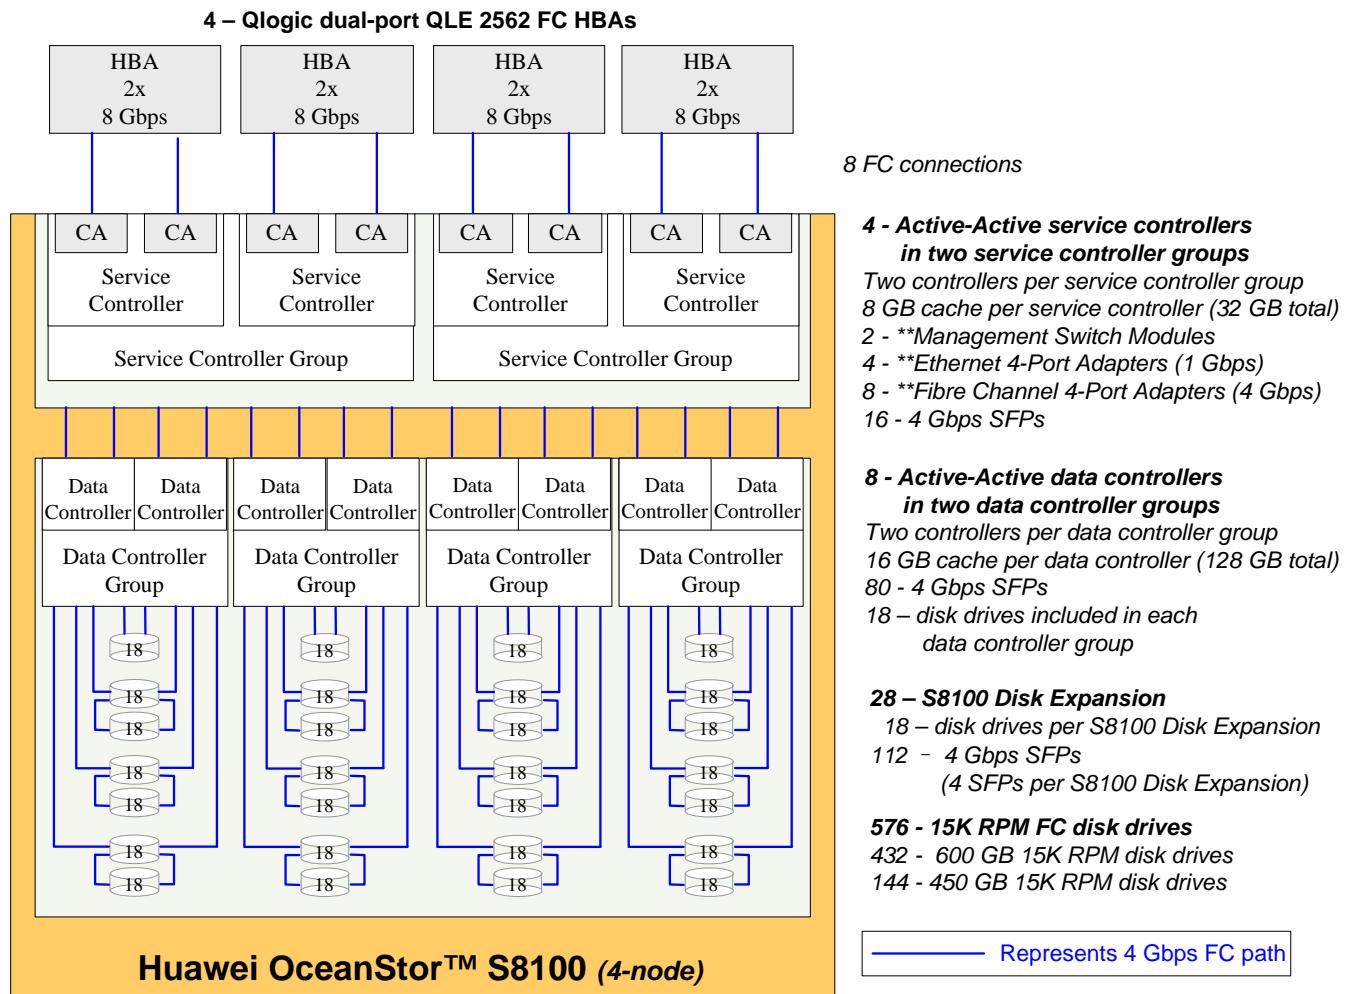

**The 2 Management Switch Modules and 4 Ethernet 4-Port Adapters are used by the service controller controllers (*nodes*) to communicate and synchronize with each other. The 8 Fibre Channel 4-Port Adapters, labeled as “CA” in the above diagram, are used by the service controllers for connectivity with the data controllers and Host Systems.

Priced Storage Configuration Components

Priced Storage Configuration:
Huawei UltraPath For Windows/Linux
4 – Qlogic dual-port QLE2562 FC HBAs
Huawei OceanStor™ S8100 (4 node)
4 - Active-Active service controllers in 2 service controller groups:
2 service controllers per service controller group
8 GB cache per service controller (<i>32 GB total</i>)
8 – Fibre Channel 4-port adapters (4 Gbps)
4 – 4 Gbps front-end connections per service controller (<i>16 total, 8 used</i>)
16 – 4 Gbps SFPs
8 - Active-Active data controllers in 4 data controller groups:
2 data controllers per data controller group
16 GB cache per data controller (<i>128 GB total</i>)
4 – 4 Gbps backend connections per data controller (<i>32 total, 32 used</i>)
80 – 4 Gbps SFPs
18 – 15K RPM FC disk drives included in each data controller group <i>(72 disk drives total)</i>
2 – Management Switch Modules
4 – Ethernet 4-Port Adapters (1 Gbps)
28– S8100 Disk Expansion each with four 4 Gbps SFPs (<i>112 SFPs total</i>) and 18 15K RPM FC disk drives (<i>504 disk drives total</i>)
576 – 15K RPM FC disk drives
432 – 600 GB 15K RPM disk drives
144 – 450 GB 15K RPM disk drives

In each of the following sections of this document, the appropriate Full Disclosure Report requirement, from the SPC-1 benchmark specification, is stated in italics followed by the information to fulfill the stated requirement.

CONFIGURATION INFORMATION

Benchmark Configuration (BC)/Tested Storage Configuration (TSC) Diagram

Clause 9.4.3.4.1

A one page Benchmark Configuration (BC)/Tested Storage Configuration (TSC) diagram shall be included in the FDR...

The Benchmark Configuration (BC)/Tested Storage Configuration (TSC) is illustrated on page 18 (Benchmark Configuration/Tested Storage Configuration Diagram).

Storage Network Configuration

Clause 9.4.3.4.1

...

5. *If the TSC contains network storage, the diagram will include the network configuration. If a single diagram is not sufficient to illustrate both the Benchmark Configuration and network configuration in sufficient detail, the Benchmark Configuration diagram will include a high-level network illustration as shown in Figure 9-8. In that case, a separate, detailed network configuration diagram will also be included as described in Clause 9.4.3.4.2.*

Clause 9.4.3.4.2

If a storage network was configured as a part of the Tested Storage Configuration and the Benchmark Configuration diagram described in Clause 9.4.3.4.1 contains a high-level illustration of the network configuration, the Executive Summary will contain a one page topology diagram of the storage network as illustrated in Figure 9-9.

The TSC did not utilize network storage.


Host System and Tested Storage Configuration (TSC) Table of Components

Clause 9.4.3.4.3

The FDR will contain a table that lists the major components of each Host System and the Tested Storage Configuration (TSC). Table 9-10 specifies the content, format, and appearance of the table.

The Host System and TSC table of components may be found on page 19 (*Host System(s) and Tested Storage Configuration Components*).

Benchmark Configuration/Tested Storage Configuration Diagram

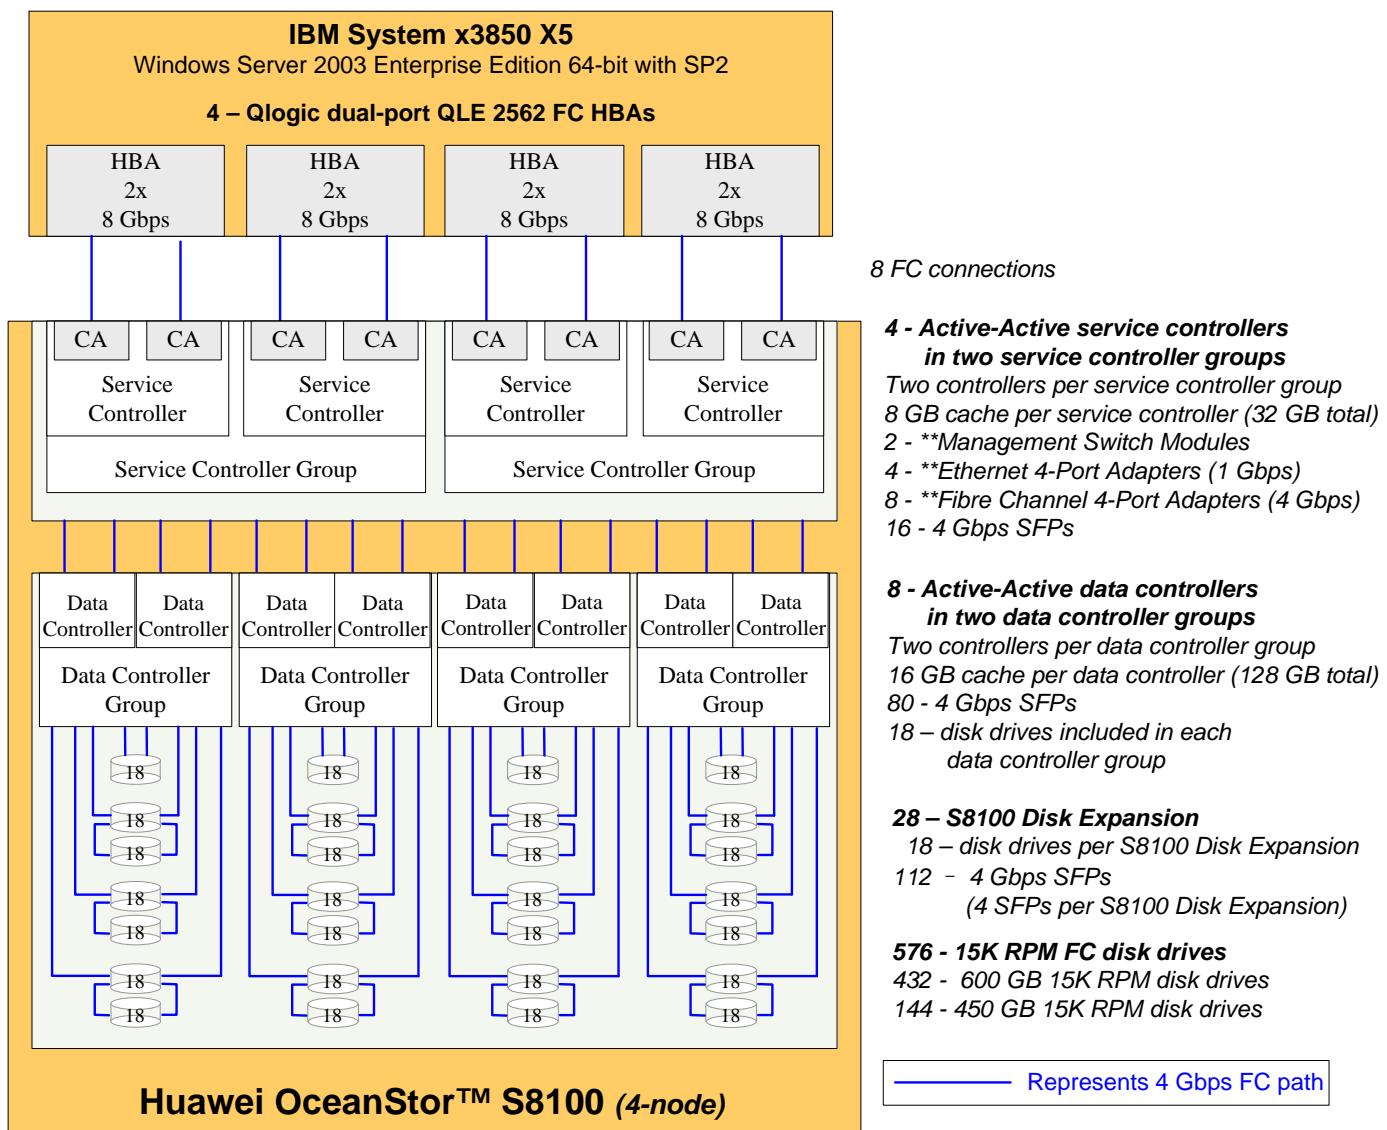

**The 2 Management Switch Modules and 4 Ethernet 4-Port Adapters are used by the service controller controllers (*nodes*) to communicate and synchronize with each other. The 8 Fibre Channel 4-Port Adapters, labeled as “CA” in the above diagram, are used by the service controllers for connectivity with the data controllers and Host Systems.

Host System(s) and Tested Storage Configuration Components

Host System:	Tested Storage Configuration (TSC):
IBM System x3850 X5 Server	Huawei UltraPath For Windows/Linux
4 – Intel Xeon E7530 1.86 GHz 6 Core Processors with 12 MB L2 cache per processor	4 – Qlogic dual-port QLE2562 FC HBAs
64 GB main memory	Huawei OceanStor™ S8100 (4 node)
Windows Server 2003 Enterprise Edition 64-bit with SP2	4 – Active-Active service controllers in 2 service controller groups 2 service controllers per service controller group 8 GB cache per service controller (<i>32 GB total</i>) 8 – Fibre Channel 4-port adapters (4 Gbps) 4 – 4 Gbps front-end connections per service controller (<i>16 total, 8 used</i>) 16 – 4 Gbps SFPs
PCIe	8 – Active-Active data controllers in 4 service controller groups 2 data controllers per data controller group 16 GB cache per data controller (<i>128 GB total</i>) 8 – Fibre Channel 4-port adapters (4 Gbps) 4 – 4 Gbps backend connections per data controller (<i>32 total, 32 used</i>) 80 – 4 Gbps SFPs 18 – 15K RPM FC disk drives included in each data controller group (<i>72 disk drives total</i>)
	2 – Management Switch Modules
	4 – Ethernet 4-Port Adapters (1 Gbps)
	28 – S8100 Disk Expansion each with four 4 Gbps SFPs (<i>112 SFPs total</i>) and 18 15K RPM FC disk drives (<i>504 disk drives total</i>)
	576 – 15K RPM FC disk drives 432 – 600 GB 15K RPM disk drives 144 – 450 GB 15K RPM disk drives

Customer Tunable Parameters and Options

Clause 9.4.3.5.1

All Benchmark Configuration (BC) components with customer tunable parameter and options that have been altered from their default values must be listed in the FDR. The FDR entry for each of those components must include both the name of the component and the altered value of the parameter or option. If the parameter name is not self-explanatory to a knowledgeable practitioner, a brief description of the parameter's use must also be included in the FDR entry.

“Appendix B: Customer Tunable Parameters and Options” on page 63 contains the customer tunable parameters and options that have been altered from their default values for this benchmark.

Tested Storage Configuration (TSC) Description

Clause 9.4.3.5.2

The FDR must include sufficient information to recreate the logical representation of the TSC. In addition to customer tunable parameters and options (Clause 4.2.4.5.3), that information must include, at a minimum:

- *A diagram and/or description of the following:*
 - *All physical components that comprise the TSC. Those components are also illustrated in the BC Configuration Diagram in Clause 9.2.4.4.1 and/or the Storage Network Configuration Diagram in Clause 9.2.4.4.2.*
 - *The logical representation of the TSC, configured from the above components that will be presented to the Workload Generator.*
- *Listings of scripts used to create the logical representation of the TSC.*
- *If scripts were not used, a description of the process used with sufficient detail to recreate the logical representation of the TSC.*

“Appendix C: Tested Storage Configuration (TSC) Creation” on page 64 contains the detailed information that describes how to create and configure the logical TSC.

SPC-1 Workload Generator Storage Configuration

Clause 9.4.3.5.3

The FDR must include all SPC-1 Workload Generator storage configuration commands and parameters.

The SPC-1 Workload Generator storage configuration commands and parameters for this measurement appear in “Appendix D: SPC-1 Workload Generator Storage Commands and Parameters” on page 72.

SPC-1 DATA REPOSITORY

This portion of the Full Disclosure Report presents the detailed information that fully documents the various SPC-1 storage capacities and mappings used in the Tested Storage Configuration. “SPC-1 Data Repository Definitions” on page 59 contains definitions of terms specific to the SPC-1 Data Repository.

Storage Capacities and Relationships

Clause 9.4.3.6.1

Two tables and an illustration documenting the storage capacities and relationships of the SPC-1 Storage Hierarchy (Clause 2.1) shall be included in the FDR.

SPC-1 Storage Capacities

SPC-1 Storage Capacities		
Storage Hierarchy Component	Units	Capacity
Total ASU Capacity	Gigabytes (GB)	92,160.000
Addressable Storage Capacity	Gigabytes (GB)	98,956.046
Configured Storage Capacity	Gigabytes (GB)	259,255.903
Physical Storage Capacity	Gigabytes (GB)	324,069.114
Data Protection (<i>Mirroring</i>)	Gigabytes (GB)	129,627.951
Required Storage (<i>metadata</i>)	Gigabytes (GB)	10.737
Global Storage Overhead	Gigabytes (GB)	239.008
Total Unused Storage	Gigabytes (GB)	139,488.632


SPC-1 Storage Hierarchy Ratios

	Addressable Storage Capacity	Configured Storage Capacity	Physical Storage Capacity
Total ASU Capacity	93.13%	35.55%	28.44%
Required for Data Protection (<i>Mirrored</i>)		50.00%	40.00%
Addressable Storage Capacity		38.17%	30.54%
Required Storage (<i>metadata</i>)		0.004%	0.003%
Configured Storage Capacity			80.00%
Global Storage Overhead			0.07%
Unused Storage:			
Addressable	6.87%		
Configured		28.90%	
Physical			19.93%

The Physical Storage Capacity consisted of 324,069.114 GB distributed over 432 disk drives each with a formatted capacity of 600.127GB and 144 disk drives, each with a formatted capacity 450.098 GB (*576 disk drives total*). There was 64,574.204 GB (19.93%) of Unused Storage within the Physical Storage Capacity. Global Storage Overhead consisted of 239.008 GB (0.07%) of Physical Storage Capacity. There was 74,914.428 GB (28.90%) of Unused Storage within the Configured Storage Capacity. The Total ASU Capacity utilized 93.13% of the Addressable Storage Capacity resulting in 6,796.046 GB (6.87%) of Unused Storage within the Addressable Storage Capacity. The Data Protection (*mirroring*) capacity was 129,627.951 GB of which 92,170.737 GB was utilized. The total Unused Storage was 139,488.632 GB.

SPC-1 Storage Capacities and Relationships Illustration

The various storage capacities configured in the benchmark result are illustrated below (*not to scale*).

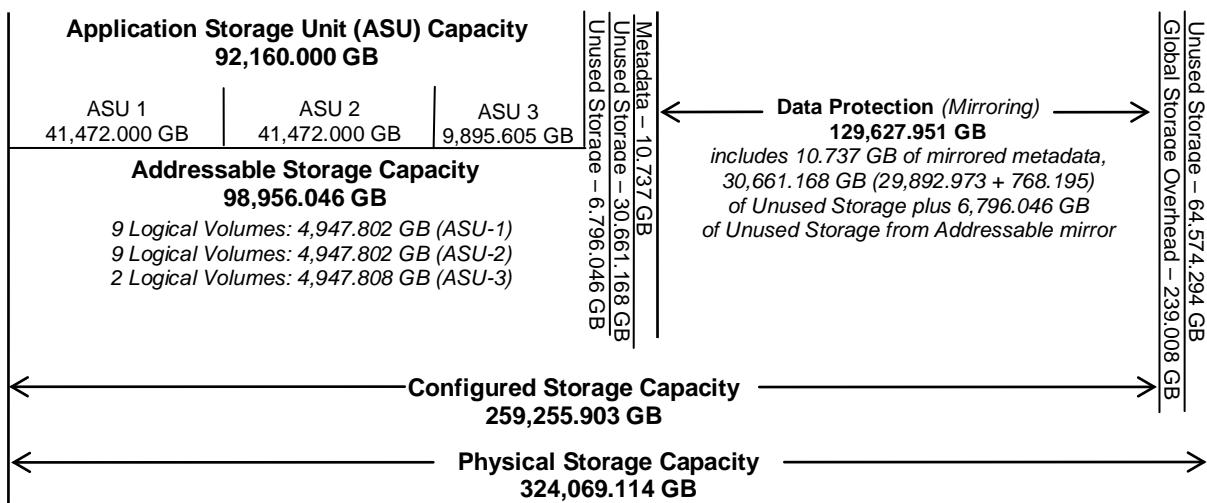

Logical Volume Capacity and ASU Mapping

Clause 9.4.3.6.3

A table illustrating the capacity of each ASU and the mapping of Logical Volumes to ASUs shall be provided in the FDR. ... Logical Volumes shall be sequenced in the table from top to bottom per its position in the contiguous address space of each ASU. The capacity of each Logical Volume shall be stated. ... In conjunction with this table, the Test Sponsor shall provide a complete description of the type of data protection (see Clause 2.4.5) used on each Logical Volume.

Logical Volume Capacity and Mapping		
ASU-1 (41,472.000 GB)	ASU-2 (41,472.000 GB)	ASU-3 (9,216.000 GB)
9 Logical Volumes 4,947.802 GB per Logical Volume (4,608.000 GB used per Logical Volume)	9 Logical Volumes 4,947.802 GB per Logical Volume (4,608.000 GB used per Logical Volume)	2 Logical Volumes 4,947.802 GB per Logical Volume (4,608.000 GB used per Logical Volume)

The Data Protection Level used for all Logical Volumes was “Mirrored” as described on page 11. See “ASU Configuration” in the [IOPS Test Results File](#) for more detailed configuration information.

Storage Capacity Utilization

Clause 9.4.3.6.2

The FDR will include a table illustrating the storage capacity utilization values defined for Application Utilization (Clause 2.8.1), Protected Application Utilization (Clause 2.8.2), and Unused Storage Ratio (Clause 2.8.3).

Clause 2.8.1

Application Utilization is defined as Total ASU Capacity divided by Physical Storage Capacity.

Clause 2.8.2

Protected Application Utilization is defined as (Total ASU Capacity plus total Data Protection Capacity minus unused Data Protection Capacity) divided by Physical Storage Capacity.

Clause 2.8.3

Unused Storage Ratio is defined as Total Unused Capacity divided by Physical Storage Capacity and may not exceed 45%.

SPC-1 Storage Capacity Utilization	
Application Utilization	28.44%
Protected Application Utilization	56.88%
Unused Storage Ratio	43.04%

SPC-1 BENCHMARK EXECUTION RESULTS

This portion of the Full Disclosure Report documents the results of the various SPC-1 Tests, Test Phases, and Test Runs. “SPC-1 Test Execution Definitions” on page 60 contains definitions of terms specific to the SPC-1 Tests, Test Phases, and Test Runs.

Clause 5.4.3

The Tests must be executed in the following sequence: Primary Metrics, Repeatability, and Data Persistence. That required sequence must be uninterrupted from the start of Primary Metrics to the completion of Persistence Test Run 1. Uninterrupted means the Benchmark Configuration shall not be power cycled, restarted, disturbed, altered, or adjusted during the above measurement sequence. If the required sequence is interrupted other than for the Host System/TSC power cycle between the two Persistence Test Runs, the measurement is invalid.

SPC-1 Tests, Test Phases, and Test Runs

The SPC-1 benchmark consists of the following Tests, Test Phases, and Test Runs:

- **Primary Metrics Test**
 - Sustainability Test Phase and Test Run
 - IOPS Test Phase and Test Run
 - Response Time Ramp Test Phase
 - 95% of IOPS Test Run
 - 90% of IOPS Test Run
 - 80% of IOPS Test Run
 - 50% of IOPS Test Run
 - 10% of IOPS Test Run (LRT)
- **Repeatability Test**
 - Repeatability Test Phase 1
 - 10% of IOPS Test Run (LRT)
 - IOPS Test Run
 - Repeatability Test Phase 2
 - 10% of IOPS Test Run (LRT)
 - IOPS Test Run
- **Data Persistence Test**
 - Data Persistence Test Run 1
 - Data Persistence Test Run 2

Each Test is an atomic unit that must be executed from start to finish before any other Test, Test Phase, or Test Run may be executed.

The results from each Test, Test Phase, and Test Run are listed below along with a more detailed explanation of each component.

Primary Metrics Test – Sustainability Test Phase

Clause 5.4.4.1.1

The Sustainability Test Phase has exactly one Test Run and shall demonstrate the maximum sustainable I/O Request Throughput within at least a continuous three (3) hour Measurement Interval. This Test Phase also serves to insure that the TSC has reached Steady State prior to reporting the final maximum I/O Request Throughput result (SPC-1 IOPSTM).

Clause 5.4.4.1.2

The computed I/O Request Throughput of the Sustainability Test must be within 5% of the reported SPC-1 IOPSTM result.

Clause 5.4.4.1.4

The Average Response Time, as defined in Clause 5.1.1, will be computed and reported for the Sustainability Test Run and cannot exceed 30 milliseconds. If the Average Response time exceeds that 30-milliseconds constraint, the measurement is invalid.

Clause 9.4.3.7.1

For the Sustainability Test Phase the FDR shall contain:

1. *A Data Rate Distribution graph and data table.*
2. *I/O Request Throughput Distribution graph and data table.*
3. *A Response Time Frequency Distribution graph and table.*
4. *An Average Response Time Distribution graph and table.*
5. *The human readable Test Run Results File produced by the Workload Generator (may be included in an appendix).*
6. *A listing or screen image of all input parameters supplied to the Workload Generator (may be included in an appendix).*
7. *The Measured Intensity Multiplier for each I/O stream.*
8. *The variability of the Measured Intensity Multiplier, as defined in Clause 5.3.13.3.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 74.

Sustainability Test Results File


A link to the test results file generated from the Sustainability Test Run is listed below.

[Sustainability Test Results File](#)

Sustainability – Data Rate Distribution Data (MB/second)

Ramp-Up/Start-Up	Start	Stop	Interval	Duration										
Measurement Interval	14:44:58	14:47:58	0-2	0:03:00										
Interval	All ASUs	ASU1	ASU2	ASU3	Interval	All ASUs	ASU1	ASU2	ASU3	Interval	All ASUs	ASU1	ASU2	ASU3
0	1,314.14	510.41	140.22	663.50	63	1,313.71	510.13	140.48	663.10	126	1,312.75	510.19	140.07	662.50
1	1,313.47	509.67	140.30	663.50	64	1,312.60	509.85	140.60	662.14	127	1,312.31	509.71	140.31	662.29
2	1,313.61	509.70	140.65	663.27	65	1,311.76	510.08	139.99	661.69	128	1,313.04	509.97	140.14	662.92
3	1,312.48	509.64	140.31	662.53	66	1,312.37	510.02	139.91	662.44	129	1,313.74	509.72	140.25	663.76
4	1,312.57	510.20	140.51	661.86	67	1,313.62	509.99	140.48	663.15	130	1,312.26	509.54	140.13	662.59
5	1,314.01	510.49	140.05	663.48	68	1,313.46	510.84	140.33	662.29	131	1,313.07	510.22	140.20	662.65
6	1,311.75	509.36	140.17	662.22	69	1,314.36	510.16	140.54	663.66	132	1,313.87	509.85	140.28	663.74
7	1,313.79	510.50	140.40	662.89	70	1,313.12	509.95	140.28	662.90	133	1,313.27	510.31	140.26	662.70
8	1,312.86	509.83	140.34	662.69	71	1,313.39	509.92	140.84	662.62	134	1,311.43	509.50	139.88	662.05
9	1,313.87	510.25	139.90	663.72	72	1,313.13	509.59	140.12	663.42	135	1,313.48	509.64	140.28	663.55
10	1,313.79	510.60	139.93	663.26	73	1,312.12	509.54	140.30	662.28	136	1,312.47	509.01	140.08	663.38
11	1,312.71	509.85	140.10	662.76	74	1,311.71	509.64	140.17	661.90	137	1,313.97	510.17	139.91	663.89
12	1,313.62	510.17	140.13	663.32	75	1,312.69	509.86	140.03	662.80	138	1,313.84	510.02	140.19	663.64
13	1,313.07	509.84	140.63	662.60	76	1,313.55	509.89	140.52	663.15	139	1,313.11	510.12	140.16	662.84
14	1,312.93	509.43	140.71	662.78	77	1,313.39	510.07	139.98	663.34	140	1,313.86	510.12	140.40	663.34
15	1,314.94	510.25	140.29	664.39	78	1,313.61	510.14	140.42	663.06	141	1,313.04	510.32	140.24	662.49
16	1,313.74	510.50	140.30	662.95	79	1,313.00	509.61	140.08	663.32	142	1,313.61	510.04	140.25	663.31
17	1,314.87	509.89	140.54	664.44	80	1,314.46	510.41	140.15	663.91	143	1,313.60	510.18	140.28	663.14
18	1,313.09	510.18	140.01	662.90	81	1,312.93	509.98	140.45	662.51	144	1,312.85	510.24	140.17	662.44
19	1,313.91	510.45	140.49	662.96	82	1,313.93	510.22	140.21	663.51	145	1,312.08	509.72	140.09	662.26
20	1,313.16	509.89	140.48	662.79	83	1,313.48	510.13	140.63	662.72	146	1,313.57	509.67	140.35	663.54
21	1,313.15	509.88	140.05	663.22	84	1,314.16	509.86	140.46	663.83	147	1,314.48	510.46	140.42	663.60
22	1,313.05	510.16	140.12	662.77	85	1,313.54	509.69	139.96	663.89	148	1,313.54	510.43	139.96	663.15
23	1,313.34	510.13	140.49	662.72	86	1,312.85	510.01	140.36	662.48	149	1,312.98	509.31	140.64	663.03
24	1,313.15	509.87	140.17	663.11	87	1,314.16	510.10	140.61	663.44	150	1,313.88	510.61	140.52	662.75
25	1,313.65	509.86	140.29	663.50	88	1,313.61	510.23	140.17	663.21	151	1,312.96	510.15	140.35	662.46
26	1,312.74	510.62	139.80	662.32	89	1,313.63	509.65	140.43	663.56	152	1,313.21	509.97	140.78	662.46
27	1,313.87	510.39	140.51	662.97	90	1,312.95	510.38	140.16	662.42	153	1,313.75	510.00	140.34	663.41
28	1,315.07	511.19	140.11	663.76	91	1,313.37	509.90	140.25	663.22	154	1,313.98	510.30	140.39	663.29
29	1,313.37	510.40	139.95	663.02	92	1,313.26	510.04	140.32	662.90	155	1,313.09	509.54	140.02	663.53
30	1,313.28	510.47	140.46	662.35	93	1,314.01	510.01	140.19	663.81	156	1,312.97	509.87	140.01	663.09
31	1,313.32	509.07	140.31	663.94	94	1,313.03	509.87	140.24	662.92	157	1,314.09	510.53	140.47	663.10
32	1,314.19	509.83	139.96	664.40	95	1,314.66	510.58	140.10	663.98	158	1,314.16	510.24	140.45	663.47
33	1,313.98	509.67	140.13	664.18	96	1,314.86	510.18	140.26	664.43	159	1,314.00	510.51	140.34	663.15
34	1,314.41	510.33	140.54	663.55	97	1,313.11	510.11	140.39	662.61	160	1,313.44	509.47	139.96	664.01
35	1,314.89	510.60	140.45	663.83	98	1,313.29	510.29	140.31	662.69	161	1,313.22	510.17	140.62	662.43
36	1,313.82	509.94	140.23	662.65	99	1,314.60	510.11	140.17	664.33	162	1,312.76	509.88	140.34	662.54
37	1,313.00	509.85	140.30	662.86	100	1,313.52	509.60	140.50	663.42	163	1,311.92	509.96	139.82	662.13
38	1,313.34	510.11	140.38	662.86	101	1,314.25	509.85	140.30	664.10	164	1,312.96	509.67	140.17	663.12
39	1,314.11	509.85	140.32	663.94	102	1,313.95	510.29	140.59	663.07	165	1,312.66	509.67	140.26	662.73
40	1,312.88	510.06	140.18	662.64	103	1,312.90	510.30	140.13	662.48	166	1,313.28	509.99	140.37	662.92
41	1,312.86	509.89	140.29	662.68	104	1,313.44	510.57	140.10	662.77	167	1,313.70	509.82	140.18	663.70
42	1,313.68	509.95	140.20	663.53	105	1,313.04	510.19	140.03	662.83	168	1,311.91	509.90	140.07	661.95
43	1,313.77	510.28	140.39	663.10	106	1,313.43	510.43	140.08	662.92	169	1,313.20	509.72	139.93	663.56
44	1,313.14	509.96	140.62	662.56	107	1,312.70	509.53	140.06	663.11	170	1,312.94	510.27	140.37	662.30
45	1,313.77	510.10	140.30	663.36	108	1,312.55	509.84	139.97	662.74	171	1,313.92	510.14	140.33	663.45
46	1,312.89	509.44	140.07	663.38	109	1,314.90	510.21	140.49	664.20	172	1,314.38	509.98	139.82	664.58
47	1,314.08	510.27	140.19	663.63	110	1,312.39	509.53	139.93	662.92	173	1,313.85	510.24	140.22	663.39
48	1,313.63	510.54	140.37	662.72	111	1,314.40	510.63	140.62	663.14	174	1,313.48	510.02	140.54	662.91
49	1,312.60	509.84	140.21	662.56	112	1,313.49	510.06	140.32	663.11	175	1,312.94	510.32	140.39	662.22
50	1,313.31	510.35	140.23	662.74	113	1,313.29	509.83	140.36	663.10	176	1,312.85	509.84	140.35	662.66
51	1,312.30	509.48	140.30	662.52	114	1,313.62	510.14	140.34	663.13	177	1,313.04	510.35	140.15	662.54
52	1,312.27	509.79	140.16	662.32	115	1,314.06	510.17	140.48	663.41	178	1,313.17	509.15	140.59	663.43
53	1,312.08	509.10	140.09	662.89	116	1,311.72	509.17	139.99	662.56	179	1,313.43	510.03	140.47	662.93
54	1,313.34	510.05	140.08	663.22	117	1,312.61	510.14	140.00	662.47	180	1,313.30	509.48	140.44	663.38
55	1,314.05	510.14	140.27	663.65	118	1,313.33	510.53	140.74	662.07	181	1,313.64	510.26	140.22	663.16
56	1,312.85	509.90	140.50	662.45	119	1,314.45	510.44	140.40	663.61	182	1,312.79	510.43	140.09	662.27
57	1,313.50	510.06	140.82	662.62	120	1,314.71	510.82	140.36	663.54					
58	1,312.74	510.03	140.24	662.47	121	1,314.23	509.61	140.40	664.22					
59	1,314.28	509.89	140.42	663.97	122	1,313.33	509.89	140.76	662.68					
60	1,313.41	510.29	140.35	662.76	123	1,312.83	509.81	139.85	663.17					
61	1,315.07	510.49	140.53	664.04	124	1,313.59	510.38	140.43	662.78					
62	1,313.36	509.85	140.26	663.26	125	1,312.38	509.44	140.21	662.73					


Sustainability – Data Rate Distribution Graph

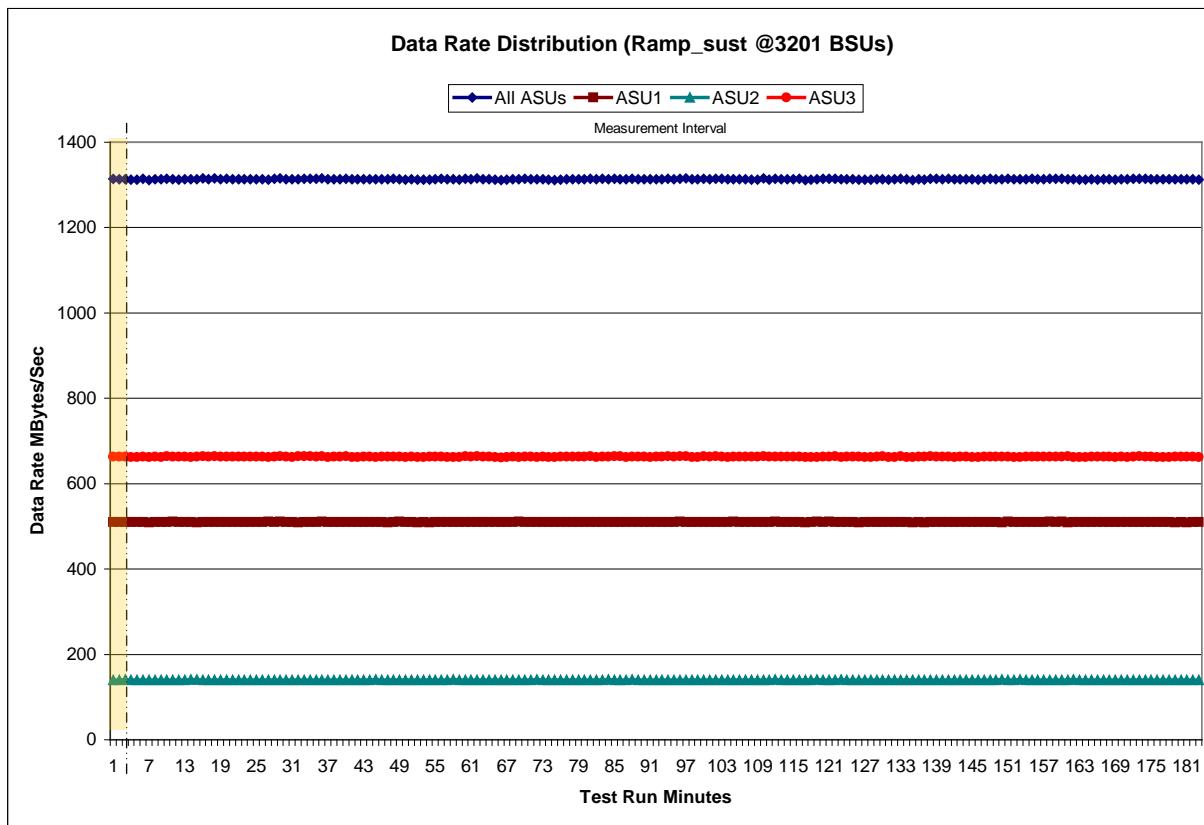

Sustainability – I/O Request Throughput Distribution Data

Ramp-Up/Start-Up		Start	Stop	Interval	Duration											
Measurement Interval		14:44:58	14:47:58	0-2	0:03:00											
		14:47:58	17:47:58	3-182	3:00:00											
Interval		All ASUs	ASU1	ASU2	ASU3	Interval	All ASUs	ASU1	ASU2	ASU3	Interval	All ASUs	ASU1	ASU2	ASU3	
0	160,285.63	95,562.92	19,694.73	45,027.98		63	160,050.13	95,366.27	19,701.18	44,982.68	126	160,019.13	95,387.67	19,700.08	44,931.38	
1	160,066.40	95,373.97	19,646.47	44,985.97		64	160,059.98	95,404.22	19,696.15	44,959.62	127	159,982.33	95,330.65	19,677.15	44,974.53	
2	160,034.57	95,400.58	19,701.28	44,932.70		65	159,956.72	95,412.38	19,644.82	44,899.52	128	160,070.55	95,402.53	19,695.82	44,972.20	
3	160,013.83	95,385.37	19,671.90	44,956.57		66	160,047.12	95,400.73	19,673.32	44,973.07	129	159,986.92	95,324.80	19,672.00	44,990.12	
4	160,074.43	95,439.57	19,725.58	44,909.28		67	160,043.13	95,370.83	19,683.65	44,988.65	130	159,946.02	95,320.38	19,663.20	44,962.43	
5	160,111.35	95,408.50	19,687.28	45,015.57		68	160,038.87	95,408.72	19,687.08	44,943.07	131	160,021.13	95,388.12	19,679.97	44,953.05	
6	159,971.97	95,334.15	19,663.07	44,974.75		69	160,111.27	95,427.97	19,682.27	45,001.03	132	160,088.80	95,390.77	19,692.73	45,005.38	
7	160,050.32	95,389.20	19,707.17	44,953.95		70	160,047.88	95,396.63	19,687.73	44,963.52	133	159,979.10	95,382.37	19,663.92	44,932.82	
8	160,021.22	95,341.72	19,681.30	44,998.20		71	160,050.70	95,381.48	19,716.67	44,952.55	134	159,930.98	95,315.90	19,683.12	44,931.97	
9	160,022.63	95,387.95	19,649.53	44,985.15		72	160,022.65	95,311.22	19,704.55	45,006.88	135	160,074.67	95,402.23	19,692.87	44,974.57	
10	160,074.53	95,405.25	19,656.62	45,012.67		73	160,005.62	95,368.58	19,691.73	44,945.30	136	159,945.72	95,316.80	19,672.60	44,954.52	
11	160,067.45	95,400.20	19,697.80	44,969.45		74	159,974.80	95,366.75	19,657.32	44,950.73	137	160,082.97	95,421.38	19,670.08	44,991.50	
12	160,046.12	95,399.25	19,655.88	44,990.98		75	159,969.43	95,351.88	19,655.93	44,961.62	138	160,009.80	95,366.02	19,673.48	44,970.30	
13	160,065.58	95,391.62	19,712.45	44,961.52		76	160,014.77	95,386.23	19,695.22	44,933.32	139	160,016.55	95,347.13	19,708.35	44,961.07	
14	160,074.50	95,357.00	19,711.78	45,005.72		77	160,069.65	95,367.58	19,700.42	45,001.65	140	160,120.77	95,424.17	19,696.02	45,000.58	
15	160,141.35	95,428.13	19,737.52	44,975.70		78	160,014.20	95,359.28	19,696.90	44,958.02	141	160,065.40	95,438.73	19,664.80	44,961.87	
16	160,111.42	95,444.45	19,683.75	44,983.22		79	160,040.98	95,326.88	19,700.60	45,013.50	142	160,026.38	95,372.92	19,684.55	44,968.92	
17	160,125.60	95,430.97	19,701.38	44,993.25		80	160,088.32	95,441.88	19,656.13	44,990.30	143	160,051.60	95,410.97	19,658.95	44,981.68	
18	160,053.75	95,414.12	19,661.02	44,978.62		81	160,061.68	95,396.87	19,685.83	44,978.98	144	160,034.42	95,382.87	19,690.20	44,961.35	
19	160,157.30	95,457.50	19,694.13	45,005.67		82	160,068.97	95,405.77	19,668.73	44,994.47	145	159,974.45	95,357.60	19,656.88	44,959.97	
20	159,987.32	95,367.68	19,694.27	44,925.37		83	160,086.27	95,414.33	19,685.50	44,986.43	146	159,997.62	95,352.52	19,681.40	44,963.70	
21	160,001.57	95,346.43	19,703.47	44,951.67		84	159,992.80	95,323.98	19,696.47	44,972.35	147	160,079.92	95,424.95	19,686.32	44,968.65	
22	160,063.82	95,427.02	19,654.00	44,982.80		85	160,072.53	95,383.62	19,683.95	45,004.97	148	160,041.88	95,430.12	19,663.23	44,954.53	
23	160,037.67	95,386.88	19,713.13	44,937.65		86	159,982.10	95,382.30	19,682.25	44,917.55	149	160,041.42	95,377.33	19,700.98	44,963.10	
24	159,984.53	95,372.95	19,670.03	44,941.55		87	160,100.88	95,397.08	19,705.67	44,998.13	150	160,096.17	95,444.80	19,704.03	44,947.33	
25	160,013.88	95,297.85	19,702.07	45,013.97		88	160,065.73	95,388.65	19,699.18	44,977.90	151	160,072.57	95,417.47	19,699.13	44,955.77	
26	160,097.37	95,464.87	19,674.95	44,957.55		89	160,014.28	95,363.88	19,687.18	44,963.22	152	160,057.70	95,368.25	19,734.75	44,954.70	
27	160,087.98	95,424.90	19,698.85	44,964.23		90	160,074.08	95,441.27	19,678.87	44,953.95	153	160,033.63	95,359.45	19,683.82	44,990.37	
28	160,158.38	95,507.50	19,678.68	44,972.20		91	160,004.80	95,365.32	19,675.58	44,963.90	154	160,098.92	95,409.02	19,713.78	44,976.12	
29	160,062.18	95,396.25	19,672.87	44,993.07		92	160,033.85	95,401.42	19,687.73	44,944.70	155	159,971.52	95,317.58	19,681.05	44,972.88	
30	160,098.68	95,433.05	19,682.05	44,983.58		93	159,988.45	95,334.07	19,672.23	44,982.15	156	159,956.02	95,340.92	19,672.13	44,942.97	
31	160,077.73	95,384.62	19,682.38	45,013.73		94	160,091.68	95,383.35	19,707.12	45,001.22	157	160,133.17	95,451.68	19,682.03	44,999.45	
32	160,029.60	95,362.87	19,646.08	45,020.65		95	160,016.85	95,364.08	19,671.05	44,981.72	158	160,134.17	95,407.80	19,716.12	45,010.25	
33	160,070.05	95,370.68	19,697.65	45,001.72		96	160,121.95	95,456.55	19,681.73	44,983.67	159	160,049.55	95,387.12	19,667.40	44,995.03	
34	160,042.25	95,396.62	19,683.98	44,961.65		97	160,050.57	95,394.02	19,684.63	44,971.92	160	160,071.15	95,393.42	19,681.32	44,996.42	
35	160,176.93	95,438.05	19,701.97	45,036.92		98	160,014.80	95,379.72	19,678.53	44,956.55	161	160,039.80	95,385.50	19,707.57	44,946.73	
36	160,003.37	95,340.33	19,685.77	44,977.27		99	160,084.48	95,395.98	19,682.52	45,005.98	162	160,031.98	95,417.48	19,703.62	44,910.88	
37	160,036.65	95,383.17	19,684.18	44,969.30		100	159,996.12	95,339.55	19,693.42	44,963.15	163	160,028.85	95,410.32	19,661.37	44,957.17	
38	160,056.58	95,402.18	19,688.77	44,965.63		101	160,023.75	95,374.97	19,686.22	44,962.57	164	160,043.03	95,381.47	19,671.40	44,990.17	
39	160,020.45	95,355.18	19,668.05	44,997.22		102	160,146.95	95,428.38	19,711.05	45,007.52	165	160,057.68	95,385.47	19,685.75	44,986.47	
40	159,973.58	95,331.23	19,683.00	44,959.35		103	160,109.33	95,450.10	19,684.90	44,974.33	166	160,127.78	95,471.92	19,686.52	44,970.35	
41	160,042.50	95,366.50	19,695.35	44,980.65		104	159,969.00	95,374.80	19,656.42	44,937.78	167	160,080.43	95,360.98	19,689.12	45,030.33	
42	160,135.45	95,436.35	19,696.07	45,003.03		105	159,994.25	95,381.35	19,659.12	44,953.78	168	159,963.03	95,338.10	19,688.23	44,936.70	
43	160,022.73	95,388.90	19,681.93	44,951.90		106	159,998.78	95,380.92	19,646.53	44,971.33	169	159,996.00	95,409.22	19,644.02	44,947.27	
44	159,990.18	95,351.02	19,691.77	44,947.40		107	159,988.62	95,351.73	19,693.82	44,943.07	170	160,045.57	95,397.75	19,689.43	44,958.38	
45	160,183.08	95,460.17	19,705.77	45,017.15		108	160,022.45	95,357.18	19,683.88	44,981.38	171	160,158.02	95,446.43	19,692.58	44,996.00	
46	159,998.97	95,379.48	19,675.70	44,949.78		109	160,082.37	95,380.70	19,705.22	44,996.45	172	160,185.77	95,457.53	19,693.88	45,034.35	
47	160,103.98	95,444.38	19,670.02	44,989.58		110	159,988.37	95,346.33	19,665.65	44,976.08	173	160,020.83	95,390.23	19,681.98	44,948.62	
48	160,001.25	95,383.60	19,693.12	44,924.53		111	160,100.60	95,471.20	19,698.12	44,931.28	174	160,146.40	95,443.47	19,705.45	44,997.48	
49	159,927.95	95,339.93	19,676.73	44,911.28		112	160,048.38	95,395.30	19,681.50	44,971.58	175	160,065.03	95,426.85	19,684.85	44,953.33	
50	160,079.18	95,433.23	19,697.18	44,948.77		113	160,007.37	95,374.92	19,682.47	44,949.98	176	160,013.38	95,377.10	19,685.17	44,951.12	
51	159,990.58	95,334.18	19,689.63	44,966.77		114	160,014.53	95,379.70	19,681.72	44,953.12	177	159,979.03	95,386.47	19,652.17	44,940.40	
52	160,038.72	95,360.90	19,679.07	44,998.75		115	160,082.22	95,392.55	19,697.70	44,991.97	178	160,042.63	95,315.49	19,700.97	45,026.22	
53	159,978.33	95,321.68	19,704.53	44,952.12		116	159,918.58	95,280.82	19,684.68	44,953.08	179	160,029.03	95,341.13	19,689.93	44,997.97	
54	160,045.85	95,388.52	19,680.70	44,975.63		117	160,066.03	95,436.95	19,662.02	44,967.07	180	160,085.95	95,359.30	19,722.18	45,004.47	
55	160,118.65	95,454.20	19,673.87	44,990.58		118	160,062.07	95,398.05	19,728.22	44,935.80	181	160,147.20	95,464.02	19,687.70	44,995.48	
56	159,989.88	95,348.03	19,720.63	44,921.22		119	160,180.62	95,481.82	19,704.03	44,994.77	182	160,026.23	95,415.77	19,690.58	44,919.88	
57	160,056.13	95,388.45	19,703.28	44,964.40		120	160,095.57	95,447.68	19,664.17	44,983.72		Average	160,046.27	95,388.68	19,685.95	44,97


Sustainability – I/O Request Throughput Distribution Graph

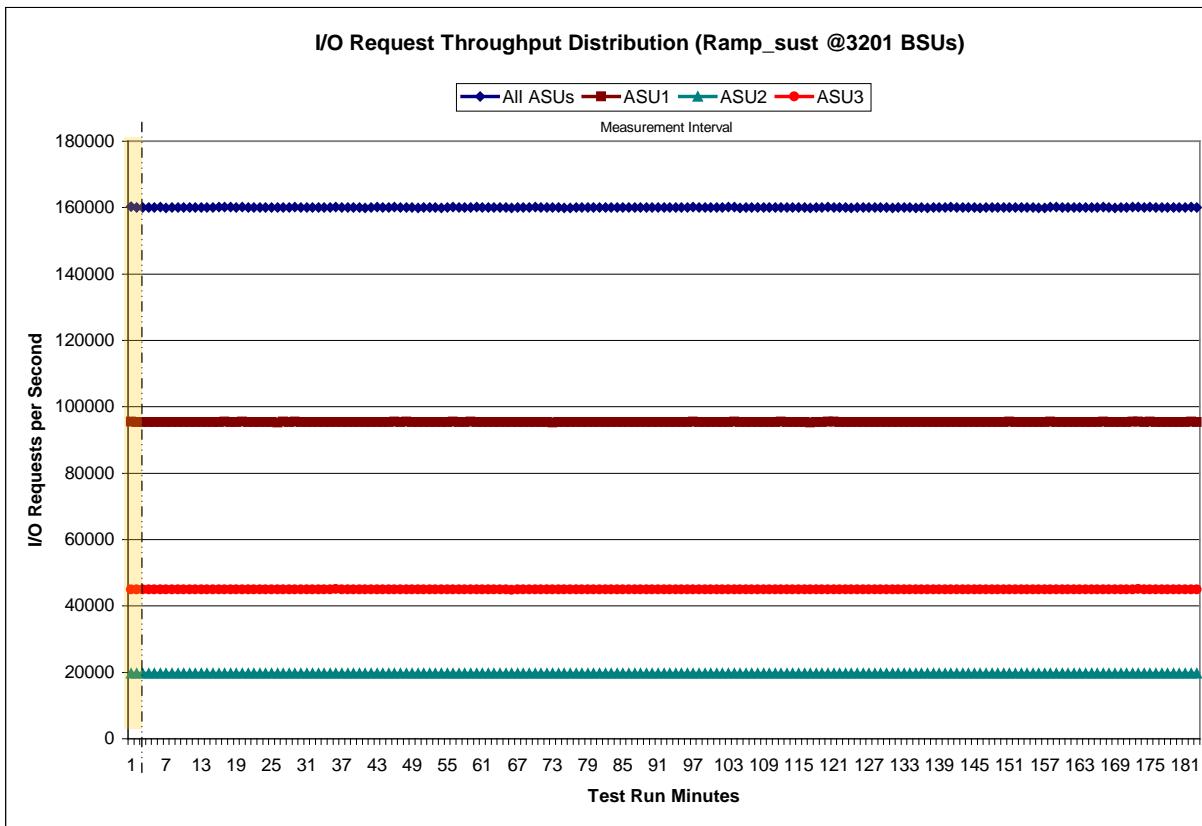

Sustainability – Average Response Time (ms) Distribution Data

Ramp-Up/Start-Up	Start	Stop	Interval	Duration										
Measurement Interval	14:44:58	14:47:58	0-2	0:03:00										
Interval	All ASUs	ASU1	ASU2	ASU3	Interval	All ASUs	ASU1	ASU2	ASU3	Interval	All ASUs	ASU1	ASU2	ASU3
0	10.87	12.65	13.70	5.84	63	9.77	12.39	14.15	2.31	126	9.81	12.43	14.13	2.35
1	9.68	12.17	13.88	2.57	64	9.75	12.35	14.05	2.35	127	9.88	12.51	14.24	2.41
2	9.72	12.27	14.09	2.41	65	9.81	12.41	14.20	2.35	128	9.89	12.55	14.30	2.32
3	9.64	12.18	14.00	2.35	66	9.77	12.36	14.08	2.40	129	9.85	12.50	14.19	2.33
4	9.62	12.18	14.01	2.25	67	9.79	12.39	14.16	2.38	130	9.79	12.41	14.12	2.32
5	9.70	12.28	14.12	2.29	68	9.81	12.43	14.16	2.36	131	9.79	12.41	14.07	2.36
6	9.54	12.08	13.87	2.27	69	9.87	12.49	14.25	2.39	132	9.96	12.59	14.35	2.46
7	9.60	12.17	13.97	2.24	70	9.75	12.36	14.02	2.35	133	9.90	12.54	14.24	2.41
8	9.66	12.23	14.03	2.32	71	9.80	12.41	14.16	2.38	134	9.90	12.55	14.31	2.36
9	9.59	12.15	13.92	2.28	72	9.87	12.50	14.26	2.38	135	9.89	12.54	14.32	2.32
10	9.69	12.25	14.06	2.34	73	9.79	12.39	14.17	2.34	136	9.90	12.56	14.33	2.32
11	9.73	12.29	14.11	2.36	74	9.72	12.29	14.03	2.36	137	9.83	12.48	14.19	2.30
12	9.79	12.36	14.17	2.41	75	9.82	12.42	14.21	2.39	138	9.92	12.58	14.34	2.34
13	9.75	12.32	14.18	2.34	76	9.80	12.41	14.20	2.31	139	9.79	12.40	14.05	2.37
14	9.69	12.25	14.09	2.32	77	9.77	12.39	14.15	2.30	140	9.94	12.59	14.30	2.43
15	9.73	12.32	14.13	2.30	78	9.72	12.33	14.13	2.25	141	9.91	12.56	14.29	2.39
16	9.63	12.20	14.04	2.26	79	9.81	12.43	14.20	2.33	142	9.92	12.58	14.34	2.37
17	9.63	12.19	13.98	2.30	80	9.84	12.49	14.23	2.31	143	10.43	13.22	15.07	2.48
18	9.73	12.28	14.04	2.43	81	9.79	12.42	14.11	2.35	144	18.24	21.75	24.17	8.19
19	9.72	12.29	14.13	2.34	82	9.72	12.31	14.02	2.34	145	9.83	12.46	14.18	2.34
20	9.69	12.27	14.07	2.29	83	9.96	12.54	14.33	2.57	146	9.91	12.55	14.26	2.40
21	9.71	12.31	14.14	2.24	84	9.80	12.41	14.16	2.36	147	9.87	12.51	14.20	2.36
22	9.73	12.32	14.14	2.31	85	9.88	12.51	14.27	2.40	148	9.86	12.49	14.17	2.38
23	9.71	12.30	14.04	2.32	86	9.82	12.43	14.16	2.37	149	9.90	12.54	14.30	2.38
24	9.75	12.33	14.12	2.34	87	9.76	12.38	14.11	2.32	150	9.89	12.54	14.27	2.33
25	9.69	12.26	14.00	2.35	88	9.92	12.58	14.34	2.35	151	9.90	12.55	14.24	2.37
26	9.73	12.29	14.06	2.40	89	9.77	12.39	14.10	2.31	152	9.93	12.59	14.34	2.36
27	9.76	12.33	14.15	2.37	90	9.77	12.37	14.01	2.38	153	9.95	12.62	14.39	2.35
28	9.82	12.40	14.20	2.40	91	9.88	12.51	14.25	2.39	154	9.91	12.58	14.31	2.33
29	9.80	12.39	14.23	2.37	92	9.91	12.53	14.28	2.43	155	9.86	12.50	14.20	2.35
30	9.70	12.27	14.04	2.34	93	9.85	12.48	14.24	2.37	156	9.85	12.49	14.18	2.37
31	9.81	12.41	14.25	2.37	94	9.93	12.56	14.33	2.43	157	9.92	12.57	14.34	2.35
32	9.73	12.32	14.07	2.34	95	9.80	12.42	14.15	2.33	158	9.85	12.50	14.18	2.35
33	9.69	12.27	14.00	2.34	96	9.91	12.56	14.35	2.34	159	9.92	12.57	14.33	2.39
34	9.72	12.27	14.03	2.40	97	9.78	12.38	14.13	2.37	160	9.94	12.61	14.31	2.37
35	9.86	12.47	14.27	2.40	98	9.81	12.42	14.12	2.39	161	9.88	12.52	14.21	2.38
36	9.66	12.23	13.96	2.35	99	9.87	12.50	14.27	2.37	162	9.94	12.61	14.30	2.35
37	9.76	12.34	14.13	2.37	100	9.94	12.57	14.39	2.40	163	9.87	12.51	14.20	2.37
38	9.76	12.35	14.18	2.35	101	9.93	12.55	14.32	2.43	164	9.88	12.53	14.22	2.35
39	9.79	12.39	14.19	2.35	102	9.89	12.53	14.26	2.41	165	10.01	12.69	14.39	2.43
40	9.72	12.31	14.06	2.32	103	9.88	12.52	14.28	2.34	166	10.00	12.67	14.43	2.40
41	9.69	12.26	13.97	2.37	104	9.84	12.49	14.22	2.33	167	9.98	12.65	14.40	2.40
42	9.79	12.37	14.17	2.42	105	9.76	12.37	14.04	2.34	168	9.87	12.53	14.24	2.30
43	9.74	12.33	14.07	2.34	106	9.79	12.39	14.12	2.37	169	9.93	12.60	14.32	2.37
44	9.70	12.27	14.02	2.34	107	9.82	12.44	14.14	2.37	170	9.93	12.59	14.34	2.36
45	9.77	12.37	14.20	2.31	108	9.88	12.51	14.24	2.40	171	9.89	12.54	14.23	2.38
46	9.77	12.37	14.17	2.31	109	9.90	12.57	14.34	2.31	172	9.92	12.60	14.30	2.34
47	9.79	12.40	14.18	2.35	110	9.85	12.50	14.23	2.33	173	9.98	12.64	14.32	2.46
48	9.84	12.47	14.26	2.32	111	10.53	13.21	14.98	2.88	174	10.02	12.69	14.45	2.40
49	9.69	12.29	13.96	2.32	112	9.87	12.53	14.27	2.30	175	9.98	12.65	14.43	2.38
50	9.74	12.31	14.04	2.40	113	9.82	12.46	14.15	2.34	176	9.97	12.65	14.39	2.35
51	9.78	12.36	14.11	2.42	114	9.84	12.46	14.16	2.39	177	9.93	12.61	14.34	2.31
52	9.79	12.38	14.12	2.42	115	9.84	12.47	14.19	2.36	178	9.87	12.56	14.28	2.26
53	9.84	12.44	14.22	2.41	116	9.84	12.46	14.15	2.39	179	9.88	12.55	14.20	2.35
54	9.81	12.43	14.18	2.35	117	9.92	12.57	14.35	2.37	180	9.90	12.55	14.25	2.38
55	9.85	12.46	14.27	2.37	118	9.90	12.53	14.26	2.39	181	9.93	12.60	14.32	2.35
56	9.88	12.51	14.30	2.36	119	9.84	12.48	14.22	2.33	182	9.94	12.62	14.30	2.35
57	9.71	12.31	14.05	2.31	120	10.02	12.72	14.53	2.33					
58	9.67	12.25	13.93	2.32	121	9.73	12.38	14.06	2.23					
59	9.82	12.41	14.17	2.41	122	9.77	12.40	14.12	2.27					
60	9.83	12.43	14.20	2.37	123	9.88	12.52	14.20	2.40					
61	9.87	12.50	14.33	2.34	124	9.96	12.61	14.38	2.40					
62	9.71	12.31	14.07	2.27	125	9.86	12.50	14.19	2.38					


Sustainability – Average Response Time (ms) Distribution Graph

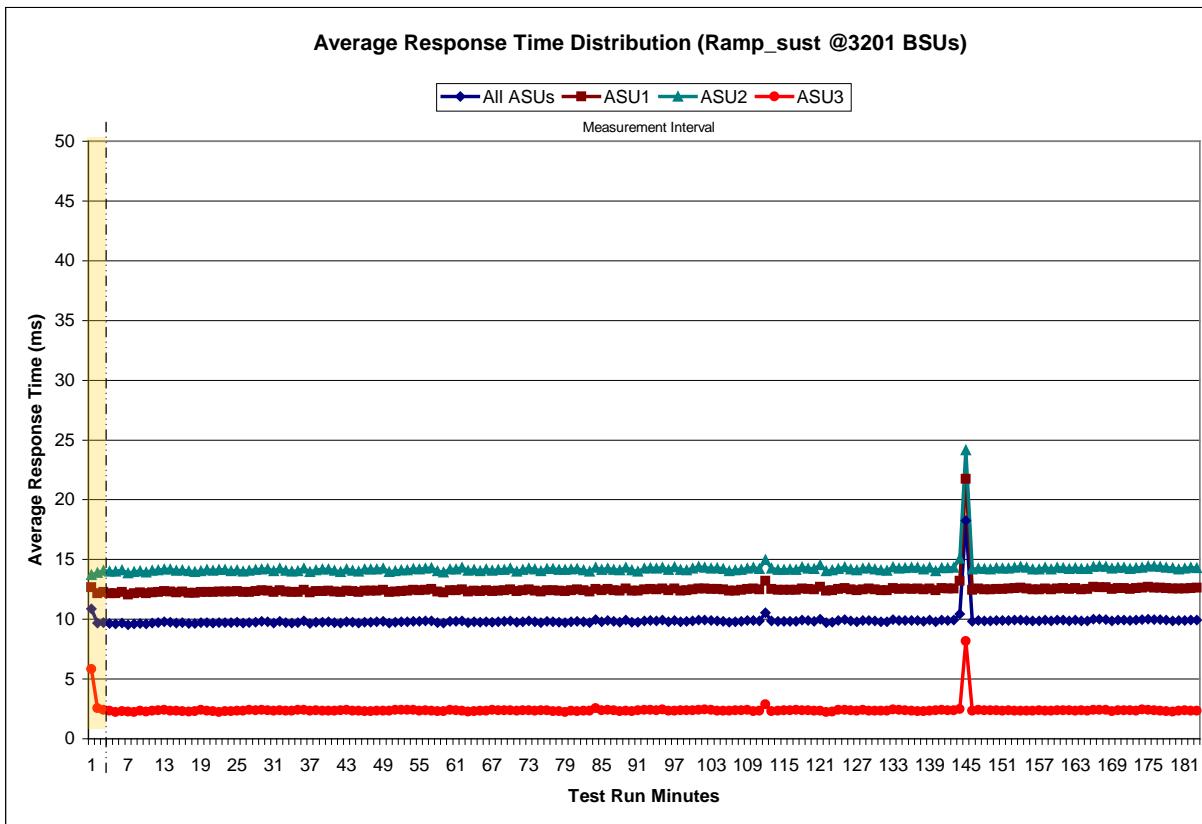

Sustainability – Response Time Frequency Distribution Data

Response Time (ms)	0-0.25	>0.25-0.5	>0.5-0.75	>0.75-1.0	>1.0-1.25	>1.25-1.5	>1.5-1.75	>1.75-2.0
Read	88,427	2,003,311	3,732,470	4,771,297	5,021,665	4,813,064	4,452,597	4,086,962
Write	18,503	30,931,393	74,070,711	87,528,259	91,903,578	93,377,357	92,172,117	88,194,473
All ASUs	106,930	32,934,704	77,803,181	92,299,556	96,925,243	98,190,421	96,624,714	92,281,435
ASU1	97,180	17,717,781	37,632,248	43,345,816	45,203,807	45,507,642	44,317,554	41,881,038
ASU2	6,126	3,782,539	8,231,738	9,497,855	9,959,041	10,110,925	9,917,588	9,401,579
ASU3	3,624	11,434,384	31,939,195	39,455,885	41,762,395	42,571,854	42,389,572	40,998,818
Response Time (ms)	>2.0-2.5	>2.5-3.0	>3.0-3.5	>3.5-4.0	>4.0-4.5	>4.5-5.0	>5.0-6.0	>6.0-7.0
Read	7,349,181	6,706,903	6,804,153	8,000,941	10,283,737	13,275,690	34,920,697	39,842,691
Write	157,311,909	123,585,689	85,378,804	51,202,077	27,269,687	14,008,216	12,167,416	5,304,397
All ASUs	164,661,090	130,292,592	92,182,957	59,203,018	37,553,424	27,283,906	47,088,113	45,147,088
ASU1	73,917,563	58,262,311	41,868,946	28,377,573	20,299,411	17,390,169	35,479,388	36,622,043
ASU2	16,595,532	12,958,792	9,038,152	5,761,263	3,749,535	2,910,405	5,567,169	5,932,152
ASU3	74,147,995	59,071,489	41,275,859	25,064,182	13,504,478	6,983,332	6,041,556	2,592,893
Response Time (ms)	>7.0-8.0	>8.0-9.0	>9.0-10.0	>10.0-15.0	>15.0-20.0	>20.0-25.0	>25.0-30.0	>30.0
Read	37,616,934	31,713,627	25,690,015	85,264,532	106,950,281	55,609,037	27,381,719	155,349,265
Write	3,119,798	1,920,097	978,775	1,372,263	1,212,631	1,192,716	431,348	2,116,700
All ASUs	40,736,732	33,633,724	26,668,790	86,636,795	108,162,912	56,801,753	27,813,067	157,465,965
ASU1	33,493,510	27,958,555	22,379,992	73,059,489	90,509,929	46,979,167	22,948,939	124,946,455
ASU2	5,725,185	4,733,207	3,795,865	12,865,244	17,020,370	9,198,935	4,639,571	31,209,194
ASU3	1,518,037	941,962	492,933	712,062	632,613	623,651	224,557	1,310,316

Sustainability – Response Time Frequency Distribution Graph

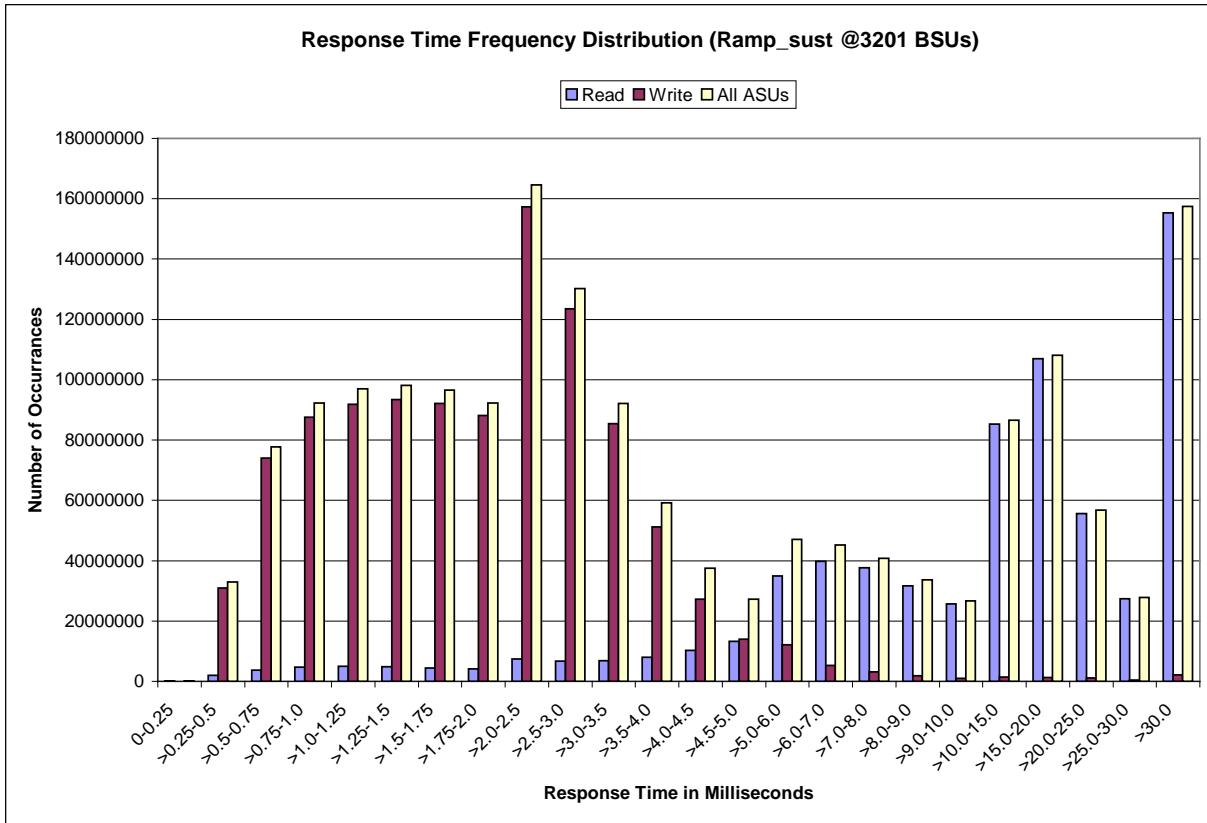

Sustainability – Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.13.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.13.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2100	0.2100	0.0180	0.0700	0.2810
COV	0.002	0.001	0.001	0.001	0.002	0.001	0.002	0.000

Primary Metrics Test – IOPS Test Phase

Clause 5.4.4.2

The IOPS Test Phase consists of one Test Run at the 100% load point with a Measurement Interval of ten (10) minutes. The IOPS Test Phase immediately follows the Sustainability Test Phase without any interruption or manual intervention.

The IOPS Test Run generates the SPC-1 IOPSTM primary metric, which is computed as the I/O Request Throughput for the Measurement Interval of the IOPS Test Run.

The Average Response Time is computed for the IOPS Test Run and cannot exceed 30 milliseconds. If the Average Response Time exceeds the 30 millisecond constraint, the measurement is invalid.

Clause 9.4.3.7.2

For the IOPS Test Phase the FDR shall contain:

1. *I/O Request Throughput Distribution (data and graph).*
2. *A Response Time Frequency Distribution.*
3. *An Average Response Time Distribution.*
4. *The human readable Test Run Results File produced by the Workload Generator.*
5. *A listing or screen image of all input parameters supplied to the Workload Generator.*
6. *The total number of I/O Requests completed in the Measurement Interval as well as the number of I/O Requests with a Response Time less than or equal to 30 milliseconds and the number of I/O Requests with a Response Time greater than 30 milliseconds.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 74.

IOPS Test Results File


A link to the test results file generated from the IOPS Test Run is listed below.

[IOPS Test Results File](#)

IOPS Test Run – I/O Request Throughput Distribution Data

3201 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	17:49:38	17:52:39	0-2	0:03:01
Measurement Interval	17:52:39	18:02:39	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	160,043.32	95,360.72	19,678.10	45,004.50
1	160,038.93	95,385.42	19,673.13	44,980.38
2	160,012.22	95,354.65	19,675.98	44,981.58
3	159,989.85	95,352.15	19,665.62	44,972.08
4	160,089.57	95,413.92	19,681.35	44,994.30
5	160,019.28	95,345.37	19,678.63	44,995.28
6	160,091.80	95,430.53	19,698.07	44,963.20
7	160,072.75	95,424.47	19,692.97	44,955.32
8	160,013.62	95,395.53	19,646.02	44,972.07
9	160,080.47	95,392.53	19,685.60	45,002.33
10	160,010.82	95,317.65	19,667.30	45,025.87
11	160,157.02	95,449.47	19,718.58	44,988.97
12	160,045.68	95,396.70	19,722.83	44,926.15
Average	160,057.09	95,391.83	19,685.70	44,979.56


IOPS Test Run – I/O Request Throughput Distribution Graph

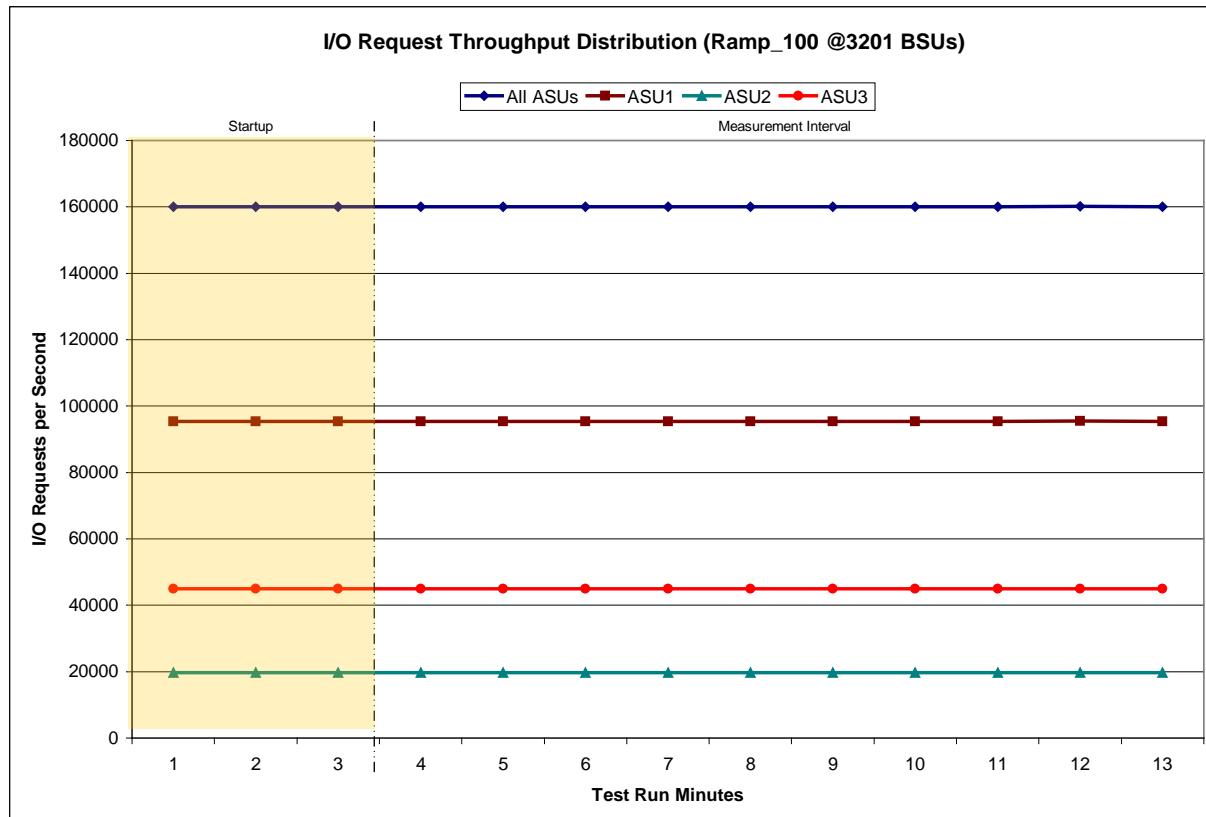

IOPS Test Run – Average Response Time (ms) Distribution Data

3201 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	17:49:38	17:52:39	0-2	0:03:01
Measurement Interval	17:52:39	18:02:39	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	10.44	12.24	13.23	5.43
1	9.34	11.84	13.50	2.23
2	9.53	12.08	13.91	2.19
3	9.47	12.03	13.86	2.13
4	9.47	12.03	13.81	2.14
5	9.50	12.05	13.86	2.17
6	9.48	12.04	13.87	2.12
7	9.45	12.01	13.81	2.11
8	9.49	12.06	13.87	2.12
9	9.43	12.00	13.82	2.07
10	9.44	12.01	13.81	2.08
11	9.46	12.03	13.85	2.10
12	9.49	12.05	13.92	2.11
Average	9.47	12.03	13.85	2.12


IOPS Test Run – Average Response Time (ms) Distribution Graph

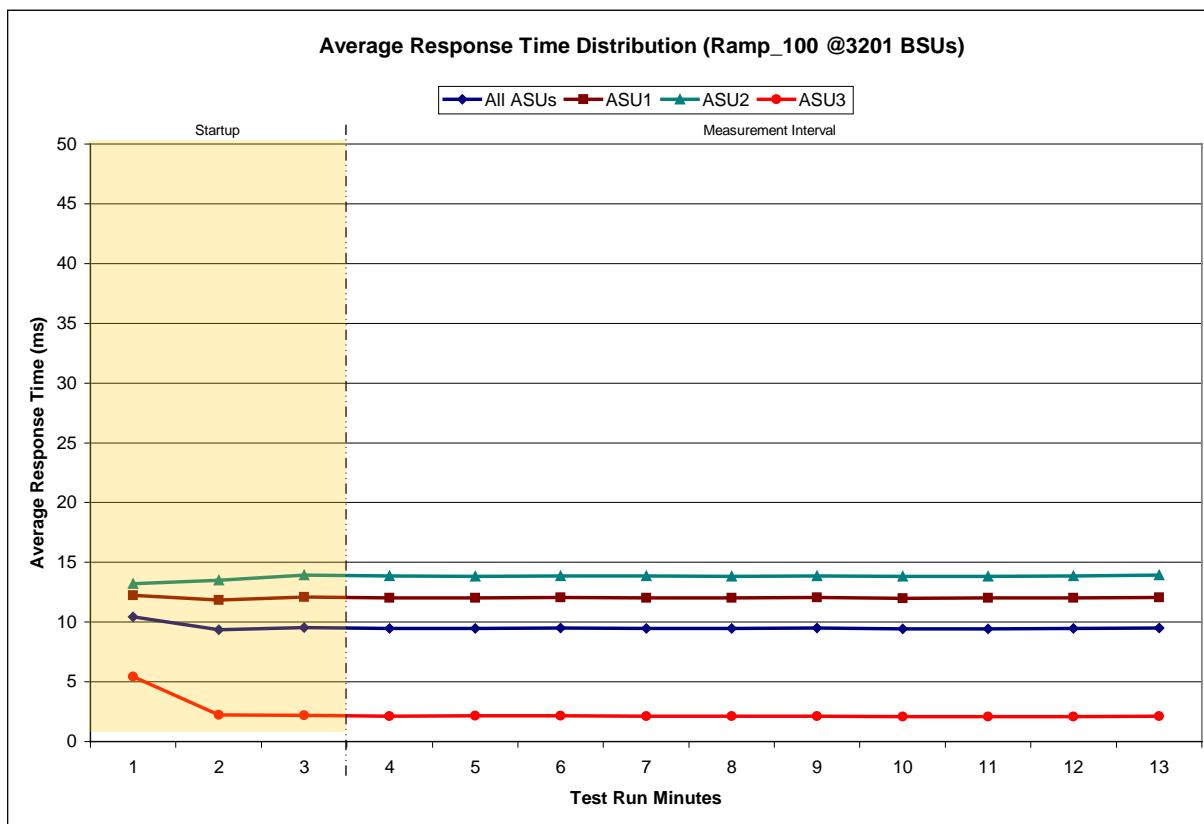

IOPS Test Run – Response Time Frequency Distribution Data

Response Time (ms)	0-0.25	>0.25-0.5	>0.5-0.75	>0.75-1.0	>1.0-1.25	>1.25-1.5	>1.5-1.75	>1.75-2.0
Read	5,488	184,006	289,896	342,025	350,005	330,180	297,167	260,503
Write	815	2,301,039	5,505,685	5,976,110	6,186,202	6,257,474	5,977,639	5,390,577
All ASUs	6,303	2,485,045	5,795,581	6,318,135	6,536,207	6,587,654	6,274,806	5,651,080
ASU1	5,820	1,362,050	2,796,139	2,959,636	3,051,525	3,039,589	2,853,008	2,535,907
ASU2	339	284,290	607,876	645,941	668,818	673,005	634,592	566,870
ASU3	144	838,705	2,391,566	2,712,558	2,815,864	2,875,060	2,787,206	2,548,303
Response Time (ms)	>2.0-2.5	>2.5-3.0	>3.0-3.5	>3.5-4.0	>4.0-4.5	>4.5-5.0	>5.0-6.0	>6.0-7.0
Read	430,462	351,840	359,114	458,843	612,844	789,489	1,998,696	2,183,517
Write	8,406,341	5,268,479	2,871,175	1,451,139	737,433	401,955	407,101	238,147
All ASUs	8,836,803	5,620,319	3,230,289	1,909,982	1,350,277	1,191,444	2,405,797	2,421,664
ASU1	3,928,223	2,509,678	1,506,685	1,005,127	843,611	857,451	1,910,074	1,980,395
ASU2	878,635	548,582	310,238	183,972	139,455	134,998	296,391	325,878
ASU3	4,029,945	2,562,059	1,413,366	720,883	367,211	198,995	199,332	115,391
Response Time (ms)	>7.0-8.0	>8.0-9.0	>9.0-10.0	>10.0-15.0	>15.0-20.0	>20.0-25.0	>25.0-30.0	>30.0
Read	2,018,802	1,693,120	1,404,619	5,200,039	5,437,172	2,930,746	1,668,075	8,275,766
Write	186,527	133,160	65,943	99,837	77,086	75,057	26,998	118,468
All ASUs	2,205,329	1,826,280	1,470,562	5,299,876	5,514,258	3,005,803	1,695,073	8,394,234
ASU1	1,801,720	1,504,043	1,227,293	4,450,079	4,597,426	2,476,675	1,394,779	6,637,052
ASU2	313,043	257,430	210,260	797,681	876,257	490,081	286,092	1,680,430
ASU3	90,566	64,807	33,009	52,116	40,575	39,047	14,202	76,752

IOPS Test Run – Response Time Frequency Distribution Graph

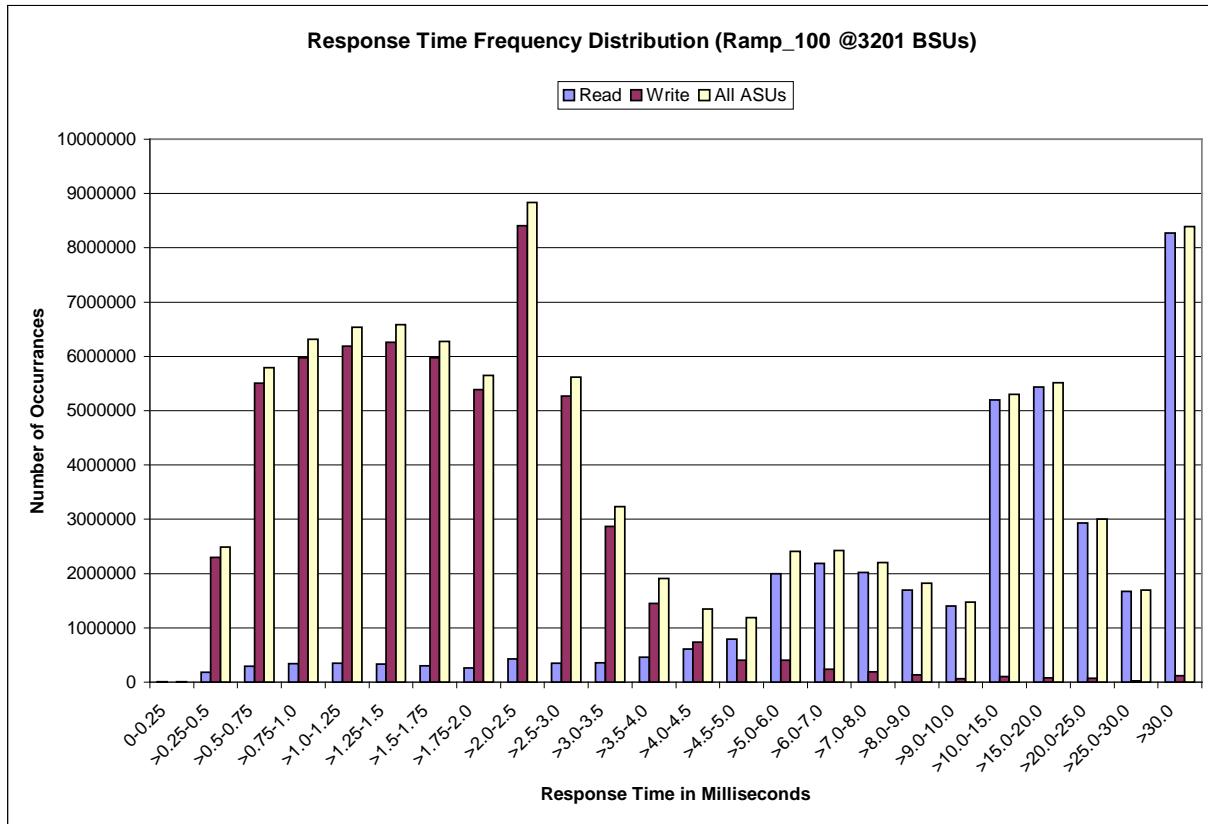

IOPS Test Run – I/O Request Information

I/O Requests Completed in the Measurement Interval	I/O Requests Completed with Response Time = or < 30 ms	I/O Requests Completed with Response Time > 30 ms
96,032,801	86,638,567	8,394,234

IOPS Test Run – Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.13.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.13.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
COV	0.002	0.000	0.001	0.000	0.004	0.001	0.002	0.001

Primary Metrics Test – Response Time Ramp Test Phase

Clause 5.4.4.3

The Response Time Ramp Test Phase consists of five Test Runs, one each at 95%, 90%, 80%, 50%, and 10% of the load point (100%) used to generate the SPC-1 IOPSTM primary metric. Each of the five Test Runs has a Measurement Interval of ten (10) minutes. The Response Time Ramp Test Phase immediately follows the IOPS Test Phase without any interruption or manual intervention.

The five Response Time Ramp Test Runs, in conjunction with the IOPS Test Run (100%), demonstrate the relationship between Average Response Time and I/O Request Throughput for the Tested Storage Configuration (TSC) as illustrated in the response time/throughput curve on page 13.

In addition, the Average Response Time measured during the 10% Test Run is the value for the SPC-1 LRT™ metric. That value represents the Average Response Time of a lightly loaded TSC.

Clause 9.4.3.7.3

The following content shall appear in the FDR for the Response Time Ramp Phase:

1. *A Response Time Ramp Distribution.*
2. *The human readable Test Run Results File produced by the Workload Generator for each Test Run within the Response Time Ramp Test Phase.*
3. *For the 10% Load Level Test Run (SPC-1 LRT™ metric) an Average Response Time Distribution.*
4. *A listing or screen image of all input parameters supplied to the Workload Generator.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 74.

Response Time Ramp Test Results File

A link to each test result file generated from each Response Time Ramp Test Run listed below.

[95% Load Level](#)

[90% Load Level](#)

[80% Load Level](#)

[50% Load Level](#)


[10% Load Level](#)

Response Time Ramp Distribution (IOPS) Data

The five Test Runs that comprise the Response Time Ramp Phase are executed at 95%, 90%, 80%, 50%, and 10% of the Business Scaling Unit (BSU) load level used to produce the SPC-1 IOPS™ primary metric. The 100% BSU load level is included in the following Response Time Ramp data tables and graphs for completeness.

100% Load Level - 3201 BSUs				95% Load Level - 3040 BSUs				Start-Up/Ramp-Up			
Measurement Interval				Measurement Interval				Measurement Interval			
(60 second intervals)				(60 second intervals)				(60 second intervals)			
0	160,043.32	95,360.72	19,678.10	45,004.50	0	151,946.18	90,599.95	18,659.65	42,686.58		
1	160,038.93	95,385.42	19,673.13	44,980.38	1	152,037.18	90,577.50	18,738.22	42,721.47		
2	160,012.22	95,354.65	19,675.98	44,981.58	2	152,064.32	90,645.25	18,697.12	42,721.95		
3	159,989.85	95,352.15	19,665.62	44,972.08	3	151,987.62	90,549.88	18,709.68	42,728.05		
4	160,089.57	95,413.92	19,681.35	44,994.30	4	152,032.53	90,616.33	18,703.97	42,712.23		
5	160,019.28	95,345.37	19,678.63	44,995.28	5	152,071.15	90,624.77	18,707.47	42,738.92		
6	160,091.80	95,430.53	19,698.07	44,963.20	6	151,987.18	90,616.55	18,692.27	42,678.37		
7	160,072.75	95,424.47	19,692.97	44,995.32	7	151,924.57	90,498.70	18,717.13	42,708.73		
8	160,013.62	95,395.53	19,646.02	44,972.07	8	151,957.00	90,590.70	18,714.23	42,652.07		
9	160,080.47	95,392.53	19,685.60	45,002.33	9	152,026.45	90,648.93	18,692.43	42,685.08		
10	160,010.82	95,317.65	19,667.30	45,025.87	10	151,967.45	90,568.68	18,710.22	42,688.55		
11	160,157.02	95,449.47	19,718.58	44,988.97	11	152,012.32	90,555.17	18,719.47	42,737.68		
12	160,045.68	95,396.70	19,722.83	44,926.15	12	152,085.90	90,654.32	18,701.52	42,730.07		
Average	160,057.09	95,391.83	19,685.70	44,979.56	Average	152,005.22	90,592.40	18,706.84	42,705.98		
90% Load Level - 2880 BSUs				80% Load Level - 2560 BSUs				Start-Up/Ramp-Up			
Measurement Interval				Measurement Interval				Measurement Interval			
(60 second intervals)				(60 second intervals)				(60 second intervals)			
0	144,000.45	85,821.37	17,702.30	40,476.78	0	127,969.43	76,287.90	15,742.73	35,938.80		
1	143,998.97	85,841.05	17,699.72	40,458.20	1	128,087.62	76,355.72	15,733.60	35,998.30		
2	144,088.33	85,862.98	17,739.70	40,485.65	2	128,009.20	76,288.52	15,761.38	35,959.30		
3	144,081.38	85,881.53	17,714.43	40,485.42	3	128,038.10	76,227.87	15,774.18	36,036.05		
4	144,059.23	85,836.75	17,692.55	40,529.93	4	128,011.87	76,276.23	15,739.12	35,996.52		
5	143,930.60	85,794.28	17,696.42	40,439.90	5	127,980.58	76,302.30	15,731.92	35,946.37		
6	144,009.40	85,841.57	17,715.78	40,452.05	6	128,028.02	76,301.30	15,739.02	35,987.70		
7	143,984.87	85,803.07	17,719.80	40,462.00	7	127,939.97	76,250.07	15,751.87	35,938.03		
8	144,017.33	85,802.43	17,748.22	40,466.68	8	127,975.10	76,287.90	15,736.93	35,950.27		
9	144,047.13	85,831.58	17,710.17	40,505.38	9	128,083.22	76,341.23	15,770.40	35,971.58		
10	144,038.58	85,840.93	17,731.57	40,466.08	10	128,041.13	76,325.27	15,736.57	35,979.30		
11	144,054.90	85,827.72	17,740.10	40,487.08	11	127,920.58	76,223.05	15,744.98	35,952.55		
12	143,936.68	85,776.43	17,712.00	40,448.25	12	127,982.95	76,289.22	15,727.30	35,966.43		
Average	144,016.01	85,823.63	17,718.10	40,474.28	Average	128,000.15	76,282.44	15,745.23	35,972.48		
50% Load Level - 1600 BSUs				Start-Up/Ramp-Up				Start-Up/Ramp-Up			
Measurement Interval				Measurement Interval				Measurement Interval			
(60 second intervals)				(60 second intervals)				(60 second intervals)			
0	80,013.55	47,722.72	9,848.33	22,442.50	0	16,019.25	9,541.38	1,973.93	4,503.93		
1	80,006.33	47,693.90	9,846.87	22,465.57	1	16,013.58	9,544.00	1,975.52	4,494.07		
2	80,063.42	47,725.92	9,834.90	22,502.60	2	16,024.62	9,551.63	1,971.02	4,501.97		
3	80,020.70	47,678.52	9,855.47	22,486.72	3	15,989.98	9,537.58	1,965.38	4,487.02		
4	79,983.78	47,642.05	9,848.18	22,493.55	4	15,990.58	9,542.35	1,961.38	4,486.85		
5	79,955.72	47,645.55	9,839.62	22,470.55	5	16,038.92	9,567.37	1,967.82	4,503.73		
6	80,073.67	47,731.85	9,846.67	22,495.15	6	16,038.10	9,557.85	1,974.30	4,505.95		
7	80,032.97	47,704.45	9,845.73	22,482.78	7	16,007.18	9,539.65	1,974.53	4,493.00		
8	79,968.45	47,644.20	9,854.27	22,469.98	8	15,991.35	9,528.15	1,967.75	4,495.45		
9	80,056.43	47,689.90	9,864.13	22,502.40	9	16,023.35	9,553.92	1,974.98	4,494.45		
10	80,008.20	47,671.62	9,838.83	22,497.75	10	15,987.90	9,539.62	1,959.22	4,489.07		
11	80,026.87	47,720.28	9,825.62	22,480.97	11	15,994.58	9,528.68	1,961.98	4,503.92		
12	80,025.70	47,673.03	9,839.15	22,513.52	12	16,004.57	9,522.15	1,979.68	4,502.73		
Average	80,015.25	47,680.15	9,845.77	22,489.34	Average	16,006.65	9,541.73	1,968.70	4,496.22		


Response Time Ramp Distribution (IOPS) Graph

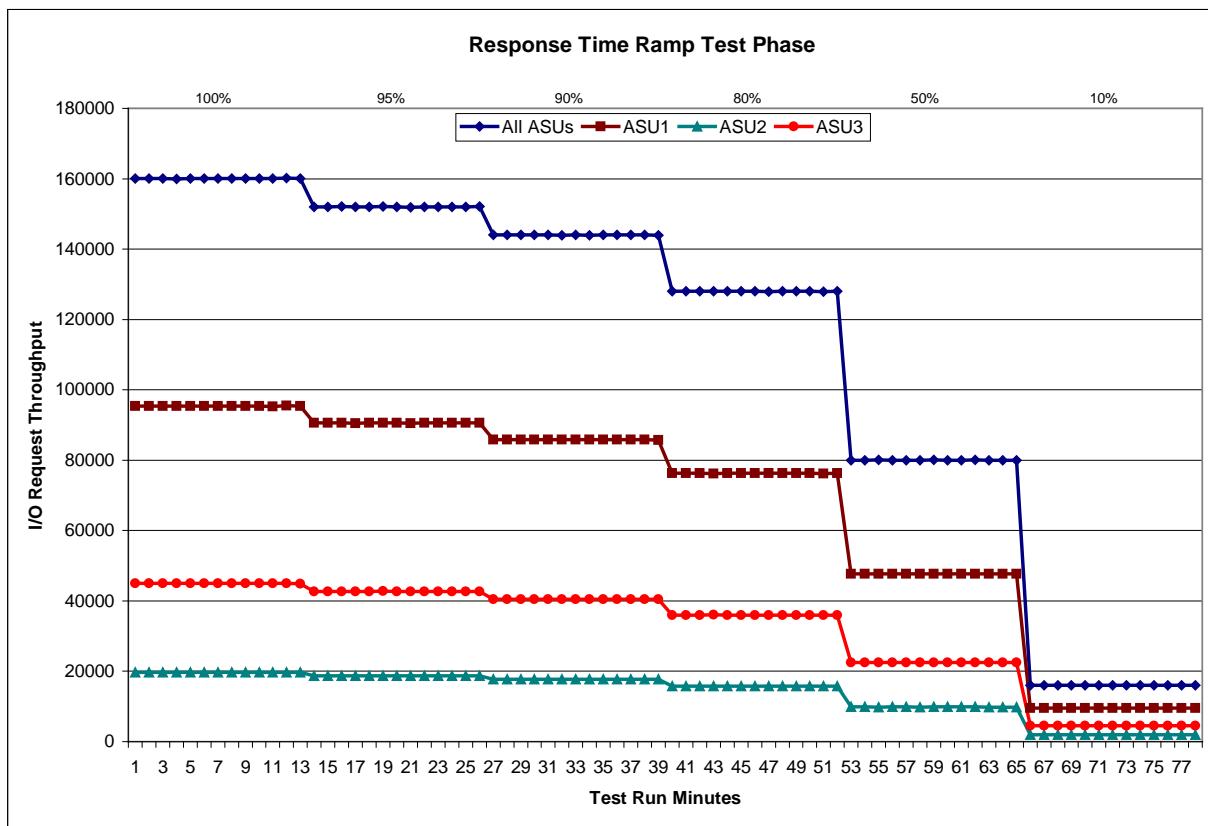

SPC-1 LRT™ Average Response Time (ms) Distribution Data

320 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	19:01:40	19:04:41	0-2	0:03:01
Measurement Interval	19:04:41	19:14:41	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	2.58	3.29	3.13	0.84
1	2.57	3.27	3.10	0.84
2	2.56	3.26	3.09	0.85
3	2.57	3.27	3.07	0.85
4	2.56	3.25	3.04	0.86
5	2.68	3.43	3.22	0.86
6	2.66	3.41	3.16	0.86
7	2.65	3.39	3.17	0.87
8	2.64	3.38	3.13	0.86
9	2.62	3.35	3.11	0.86
10	2.61	3.33	3.10	0.86
11	2.59	3.31	3.08	0.86
12	2.59	3.31	3.08	0.86
Average	2.62	3.34	3.11	0.86

SPC-1 LRT™ Average Response Time (ms) Distribution Graph

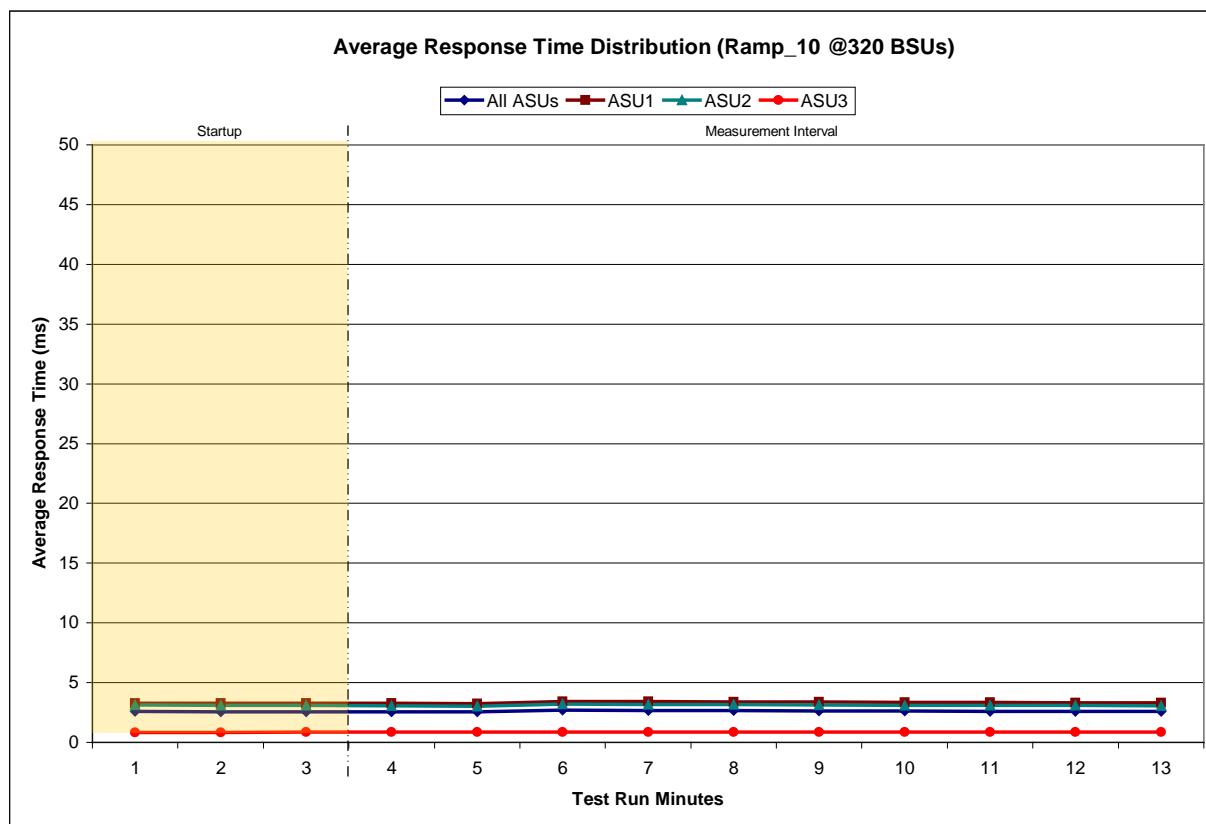

SPC-1 LRT™ (10%) – Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.13.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.13.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0349	0.2813	0.0700	0.2099	0.0181	0.0700	0.0349	0.2809
COV	0.005	0.002	0.003	0.003	0.005	0.004	0.004	0.001

Repeatability Test

Clause 5.4.5

The Repeatability Test demonstrates the repeatability and reproducibility of the SPC-1 IOPS™ primary metric and SPC-1 LRT™ metric generated in earlier Test Runs.

There are two identical Repeatability Test Phases. Each Test Phase contains two Test Runs. Each of the Test Runs will have a Measurement Interval of no less than ten (10) minutes. The two Test Runs in each Test Phase will be executed without interruption or any type of manual intervention.

The first Test Run in each Test Phase is executed at the 10% load point. The Average Response Time from each of the Test Runs is compared to the SPC-1 LRT™ metric. Each Average Response Time value must be less than the SPC-1 LRT™ metric plus 5% or less than the SPC-1 LRT™ metric plus one (1) millisecond (ms).

The second Test Run in each Test Phase is executed at the 100% load point. The I/O Request Throughput from the Test Runs is compared to the SPC-1 IOPS™ primary metric. Each I/O Request Throughput value must be greater than the SPC-1 IOPS™ primary metric minus 5%. In addition, the Average Response Time for each Test Run cannot exceed 30 milliseconds.

If any of the above constraints are not met, the benchmark measurement is invalid.

Clause 9.4.3.7.4

The following content shall appear in the FDR for each Test Run in the two Repeatability Test Phases:

1. *A table containing the results of the Repeatability Test.*
2. *An I/O Request Throughput Distribution graph and table.*
3. *An Average Response Time Distribution graph and table.*
4. *The human readable Test Run Results File produced by the Workload Generator.*
5. *A listing or screen image of all input parameters supplied to the Workload Generator.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 74.

Repeatability Test Results File

The values for the SPC-1 IOPS™, SPC-1 LRT™, and the Repeatability Test measurements are listed in the tables below.

	SPC-1 IOPS™
Primary Metrics	160,057.09
Repeatability Test Phase 1	160,044.51
Repeatability Test Phase 2	160,045.84

The SPC-1 IOPS™ values in the above table were generated using 100% of the specified Business Scaling Unit (BSU) load level. Each of the Repeatability Test Phase values for SPC-1 IOPS™ must greater than 95% of the reported SPC-1 IOPS™ Primary Metric.

	SPC-1 LRT™
Primary Metrics	2.62 ms
Repeatability Test Phase 1	2.56 ms
Repeatability Test Phase 2	2.59 ms

The average response time values in the SPC-1 LRT™ column were generated using 10% of the specified Business Scaling Unit (BSU) load level. Each of the Repeatability Test Phase values for SPC-1 LRT™ must be less than 105% of the reported SPC-1 LRT™ Primary Metric or less than the reported SPC-1 LRT™ Primary Metric minus one (1) millisecond (ms)..


A link to the test result file generated from each Repeatability Test Run is listed below.

- [Repeatability Test Phase 1, Test Run 1 \(LRT\)](#)
- [Repeatability Test Phase 1, Test Run 2 \(IOPS\)](#)
- [Repeatability Test Phase 2, Test Run 1 \(LRT\)](#)
- [Repeatability Test Phase 2, Test Run 2 \(IOPS\)](#)

Repeatability 1 LRT – I/O Request Throughput Distribution Data

320 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	19:16:11	19:19:11	0-2	0:03:00
Measurement Interval	19:19:11	19:29:13	3-12	0:10:02
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	16,028.60	9,558.58	1,973.83	4,496.18
1	15,986.00	9,524.45	1,971.57	4,489.98
2	15,993.45	9,524.40	1,969.60	4,499.45
3	15,982.73	9,525.88	1,971.97	4,484.88
4	16,044.13	9,562.07	1,969.65	4,512.42
5	16,001.97	9,533.43	1,979.27	4,489.27
6	16,015.50	9,553.65	1,969.00	4,492.85
7	16,036.23	9,563.35	1,963.83	4,509.05
8	15,989.43	9,533.83	1,964.12	4,491.48
9	16,004.60	9,542.82	1,966.40	4,495.38
10	16,022.85	9,555.50	1,967.78	4,499.57
11	16,014.68	9,547.02	1,971.27	4,496.40
12	15,997.03	9,539.63	1,975.78	4,481.62
Average	16,010.92	9,545.72	1,969.91	4,495.29


Repeatability 1 LRT – I/O Request Throughput Distribution Graph

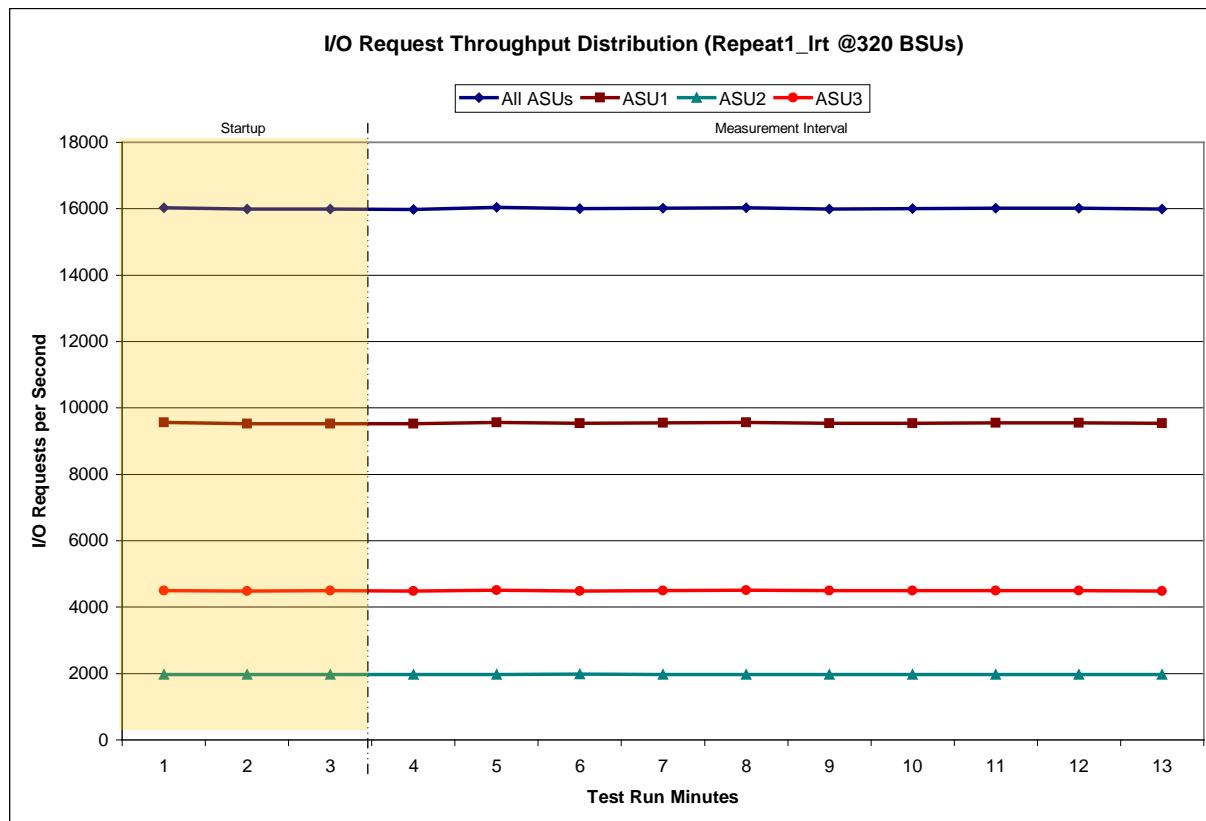

Repeatability 1 LRT –Average Response Time (ms) Distribution Data

320 BSUs	Start	Stop	Interval	Duration
<i>Start-Up/Ramp-Up</i>	19:16:11	19:19:11	0-2	0:03:00
<i>Measurement Interval</i>	19:19:11	19:29:13	3-12	0:10:02
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	2.50	3.19	2.96	0.81
1	2.49	3.17	2.95	0.82
2	2.47	3.15	2.95	0.81
3	2.46	3.15	2.90	0.81
4	2.46	3.14	2.90	0.82
5	2.59	3.33	3.10	0.82
6	2.59	3.31	3.10	0.82
7	2.59	3.32	3.13	0.83
8	2.58	3.30	3.09	0.82
9	2.57	3.29	3.06	0.82
10	2.58	3.30	3.07	0.83
11	2.57	3.29	3.05	0.82
12	2.57	3.28	3.08	0.82
Average	2.56	3.27	3.05	0.82


Repeatability 1 LRT –Average Response Time (ms) Distribution Graph

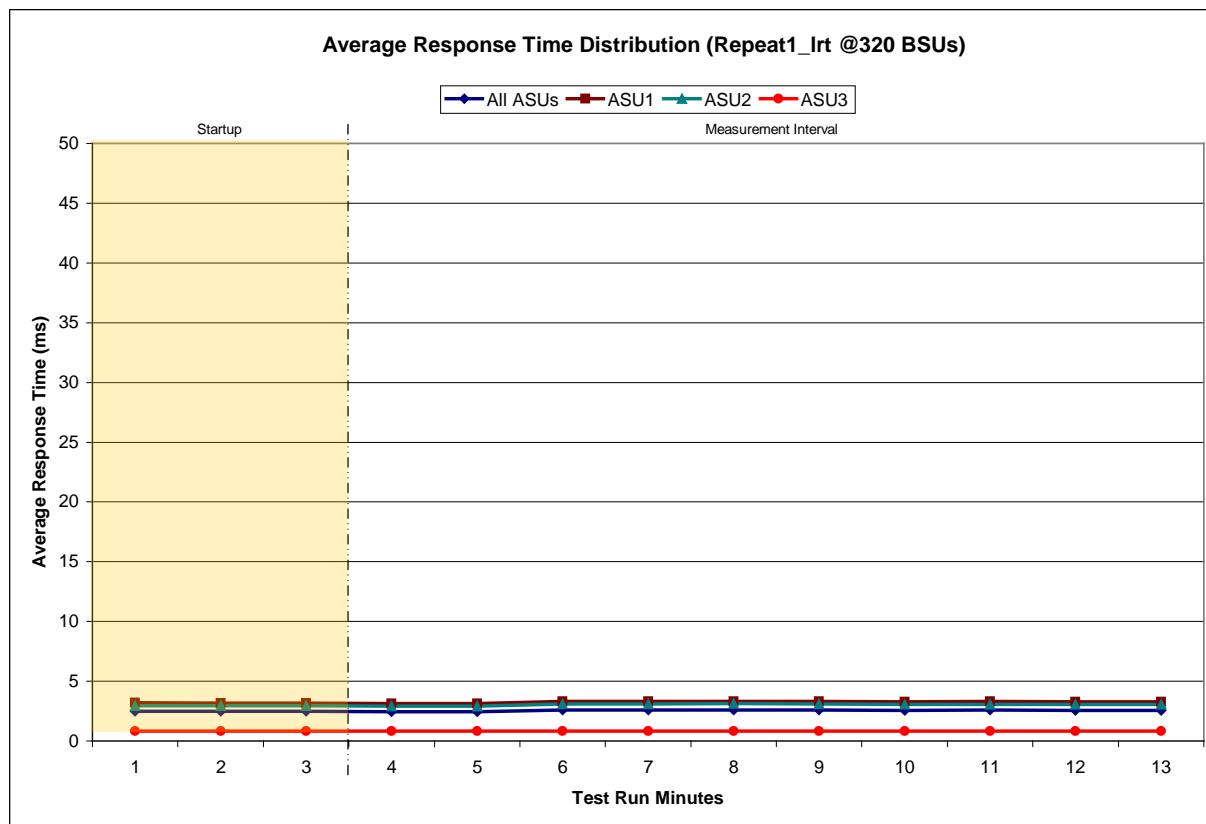

Repeatability 1 IOPS – I/O Request Throughput Distribution Data

3201 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	19:30:51	19:33:52	0-2	0:03:01
Measurement Interval	19:33:52	19:43:52	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	160,073.68	95,403.77	19,701.02	44,968.90
1	160,063.32	95,407.53	19,684.97	44,970.82
2	159,972.05	95,389.90	19,659.80	44,922.35
3	159,990.35	95,361.27	19,678.62	44,950.47
4	160,078.50	95,407.38	19,671.28	44,999.83
5	160,064.85	95,417.30	19,679.07	44,968.48
6	159,997.08	95,352.37	19,694.43	44,950.28
7	160,020.65	95,417.18	19,670.87	44,932.60
8	160,037.40	95,355.48	19,675.37	45,006.55
9	160,019.82	95,375.03	19,708.30	44,936.48
10	160,106.03	95,408.42	19,683.35	45,014.27
11	160,004.22	95,365.47	19,710.90	44,927.85
12	160,126.23	95,447.02	19,709.33	44,969.88
Average	160,044.51	95,390.69	19,688.15	44,965.67

Repeatability 1 IOPS – I/O Request Throughput Distribution Graph

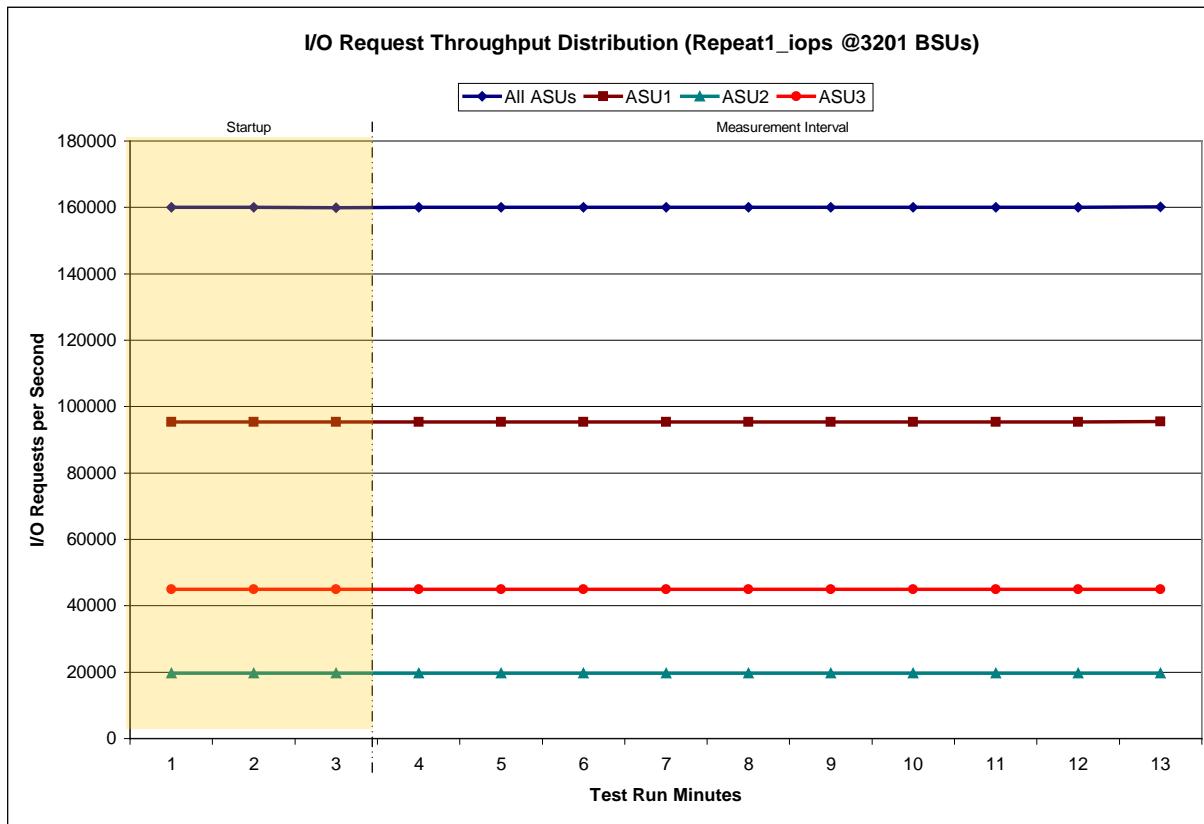

Repeatability 1 IOPS –Average Response Time (ms) Distribution Data

3201 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	19:30:51	19:33:52	0-2	0:03:01
Measurement Interval	19:33:52	19:43:52	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	15.74	17.32	18.28	11.26
1	9.37	11.86	13.56	2.25
2	9.43	11.99	13.75	2.12
3	9.50	12.06	13.91	2.13
4	9.46	12.02	13.86	2.12
5	9.48	12.03	13.84	2.15
6	9.46	11.98	13.79	2.21
7	9.54	12.10	13.93	2.19
8	9.54	12.12	13.92	2.17
9	9.57	12.15	14.03	2.15
10	9.48	12.05	13.89	2.10
11	9.53	12.11	14.00	2.10
12	9.43	11.99	13.83	2.07
Average	9.50	12.06	13.90	2.14


Repeatability 1 IOPS –Average Response Time (ms) Distribution Graph



Repeatability 2 LRT – I/O Request Throughput Distribution Data

320 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	19:45:27	19:48:27	0-2	0:03:00
Measurement Interval	19:48:27	19:58:27	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	16,028.38	9,555.77	1,966.65	4,505.97
1	16,023.45	9,549.25	1,971.03	4,503.17
2	15,982.93	9,530.70	1,962.15	4,490.08
3	16,009.37	9,533.08	1,972.03	4,504.25
4	16,015.02	9,543.32	1,975.85	4,495.85
5	15,987.98	9,529.78	1,973.28	4,484.92
6	15,975.83	9,517.22	1,963.15	4,495.47
7	15,998.82	9,524.45	1,975.10	4,499.27
8	16,023.50	9,565.83	1,966.27	4,491.40
9	15,982.22	9,527.90	1,964.78	4,489.53
10	15,990.40	9,532.80	1,966.12	4,491.48
11	16,004.38	9,532.32	1,957.62	4,514.45
12	15,977.67	9,513.63	1,959.25	4,504.78
Average	15,996.52	9,532.03	1,967.35	4,497.14


Repeatability 2 LRT – I/O Request Throughput Distribution Graph

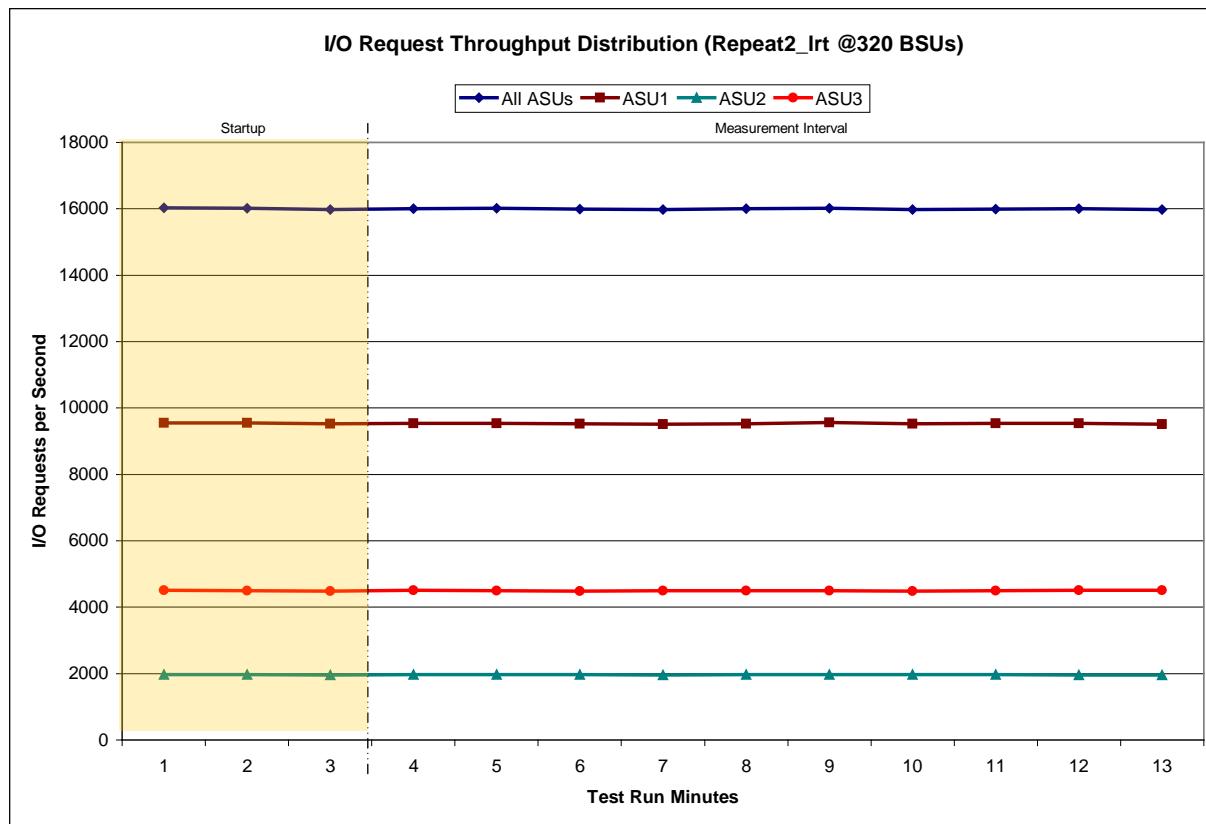

Repeatability 2 LRT –Average Response Time (ms) Distribution Data

320 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	19:45:27	19:48:27	0-2	0:03:00
Measurement Interval	19:48:27	19:58:27	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	2.59	3.30	3.17	0.82
1	2.57	3.27	3.14	0.81
2	2.56	3.27	3.13	0.82
3	2.56	3.26	3.10	0.83
4	2.55	3.25	3.07	0.82
5	2.67	3.42	3.24	0.82
6	2.63	3.36	3.19	0.83
7	2.62	3.36	3.14	0.83
8	2.60	3.33	3.12	0.83
9	2.57	3.29	3.10	0.83
10	2.57	3.28	3.08	0.83
11	2.57	3.29	3.08	0.82
12	2.57	3.28	3.09	0.83
Average	2.59	3.31	3.12	0.82


Repeatability 2 LRT –Average Response Time (ms) Distribution Graph

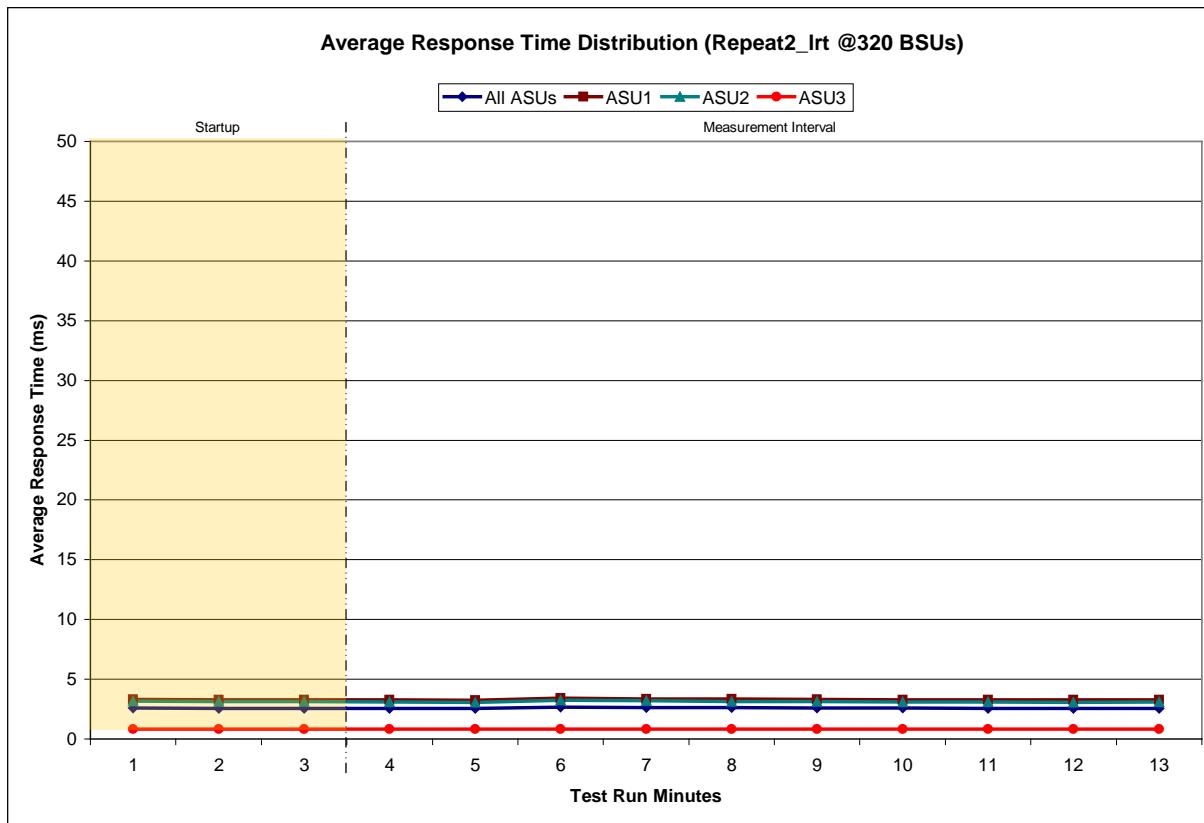

Repeatability 2 IOPS – I/O Request Throughput Distribution Data

3201 BSUs	Start	Stop	Interval	Duration
<i>Start-Up/Ramp-Up</i>	19:59:59	20:03:00	0-2	0:03:01
<i>Measurement Interval</i>	20:03:00	20:13:00	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	160,126.83	95,455.08	19,691.05	44,980.70
1	159,970.98	95,352.88	19,672.10	44,946.00
2	159,978.42	95,287.78	19,682.72	45,007.92
3	160,070.13	95,428.50	19,678.95	44,962.68
4	160,036.85	95,359.47	19,676.35	45,001.03
5	160,082.85	95,403.28	19,678.55	45,001.02
6	160,034.77	95,388.90	19,688.13	44,957.73
7	160,074.58	95,372.65	19,725.78	44,976.15
8	160,000.60	95,361.25	19,660.77	44,978.58
9	160,092.65	95,389.10	19,720.68	44,982.87
10	160,122.15	95,456.20	19,692.77	44,973.18
11	159,932.78	95,337.62	19,665.97	44,929.20
12	160,011.03	95,393.90	19,651.67	44,965.47
Average	160,045.84	95,389.09	19,683.96	44,972.79


Repeatability 2 IOPS – I/O Request Throughput Distribution Graph

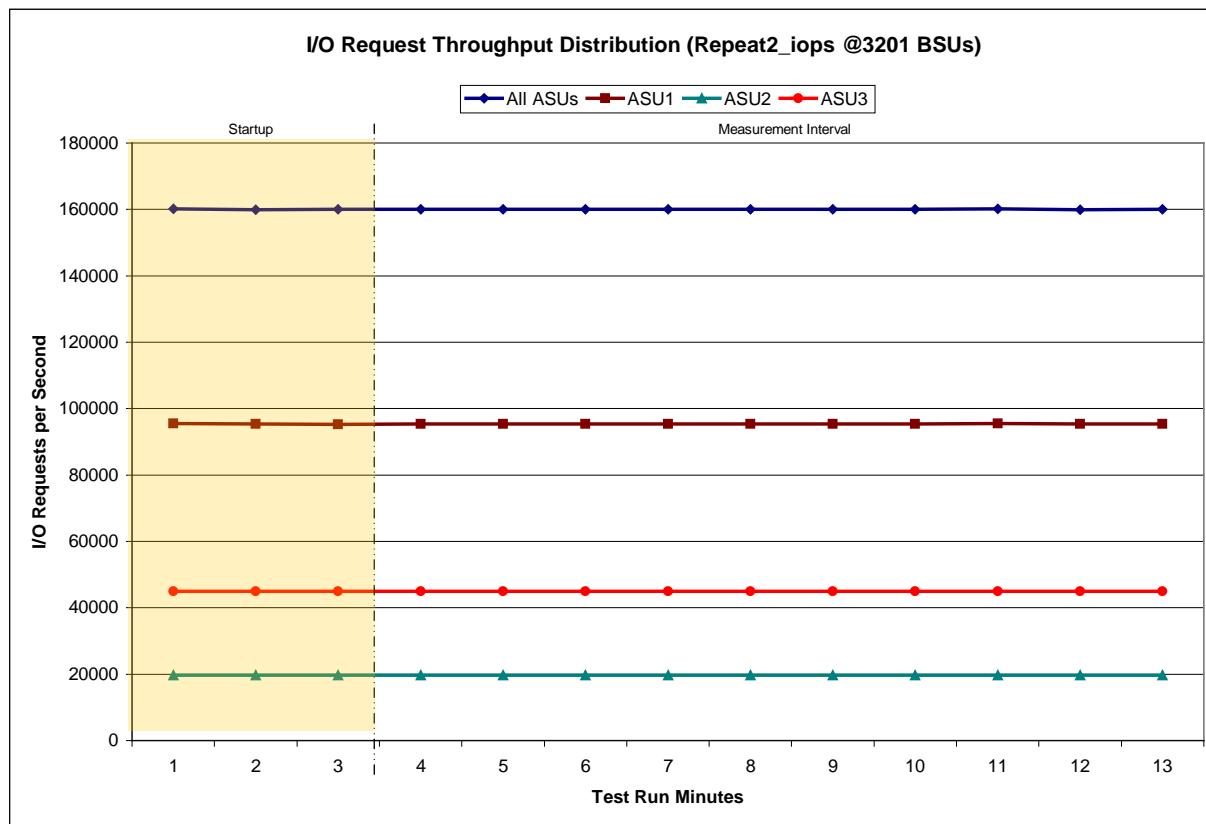

Repeatability 2 IOPS –Average Response Time (ms) Distribution Data

3201 BSUs	Start	Stop	Interval	Duration
<i>Start-Up/Ramp-Up</i>	19:59:59	20:03:00	0-2	0:03:01
<i>Measurement Interval</i>	20:03:00	20:13:00	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	13.70	15.34	16.21	9.11
1	9.35	11.84	13.56	2.22
2	9.45	11.99	13.82	2.16
3	9.47	12.04	13.90	2.07
4	9.39	11.95	13.76	2.06
5	9.52	12.10	13.96	2.10
6	9.34	11.88	13.68	2.06
7	9.48	12.07	13.95	2.05
8	9.41	11.98	13.82	2.05
9	9.43	12.00	13.81	2.05
10	9.53	12.12	13.95	2.09
11	9.56	12.17	14.02	2.10
12	9.38	11.96	13.72	2.02
Average	9.45	12.03	13.86	2.07

Repeatability 2 IOPS –Average Response Time (ms) Distribution Graph

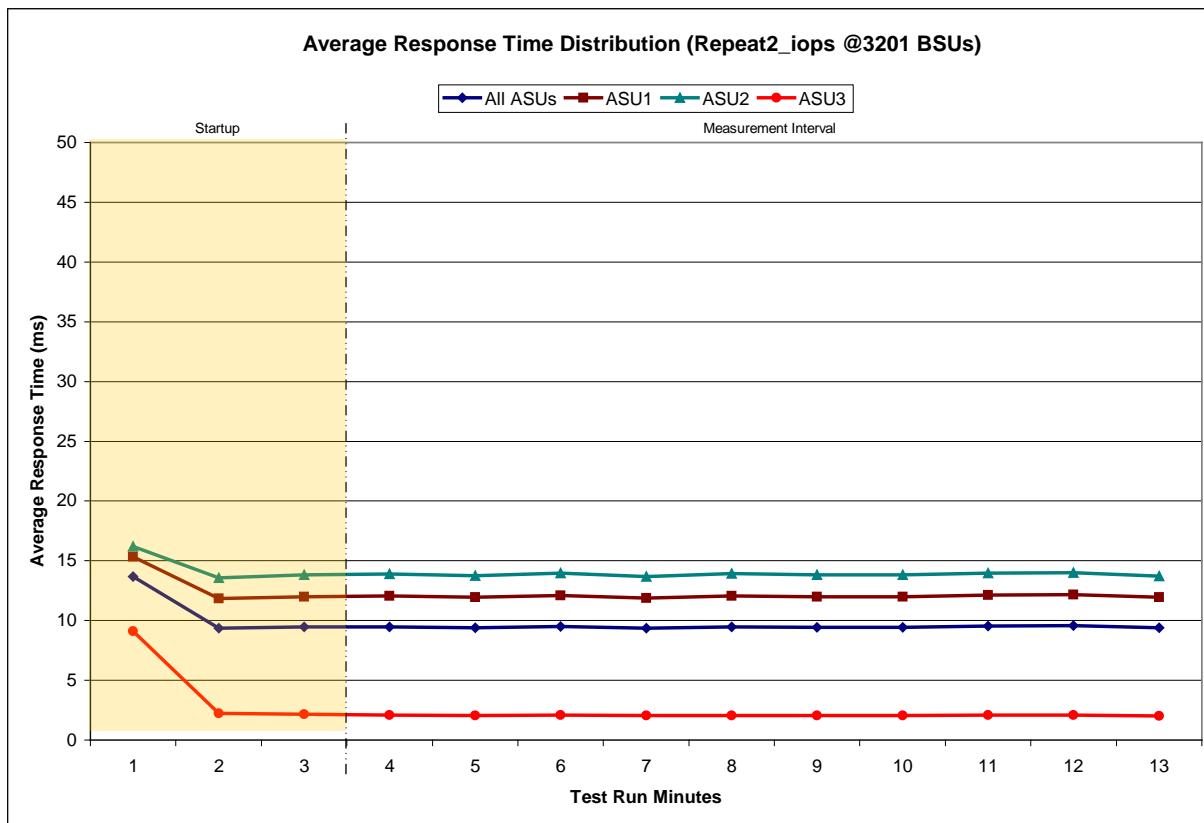

Repeatability 1 (LRT)

Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.13.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.13.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2102	0.0180	0.0700	0.0350	0.2808
COV	0.005	0.002	0.003	0.002	0.006	0.004	0.005	0.001

Repeatability 1 (IOPS)

Measured Intensity Multiplier and Coefficient of Variation

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2809	0.0700	0.2101	0.0180	0.0700	0.0350.	0.2810
COV	0.002	0.000	0.001	0.000	0.002	0.001	0.002	0.001

Repeatability 2 (LRT)

Measured Intensity Multiplier and Coefficient of Variation

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0349	0.2809	0.0700	0.2101	0.0180	0.0700	0.0349	0.2811
COV	0.006	0.002	0.005	0.002	0.008	0.004	0.007	0.002

Repeatability 2 (IOPS)
Measured Intensity Multiplier and Coefficient of Variation

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
<i>IM</i>	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
COV	0.002	0.000	0.001	0.001	0.002	0.001	0.002	0.000

Data Persistence Test

Clause 6

The Data Persistence Test demonstrates the Tested Storage Configuration (TSC):

- Is capable of maintaining data integrity across a power cycle.
- Ensures the transfer of data between Logical Volumes and host systems occurs without corruption or loss.

The SPC-1 Workload Generator will write 16 block I/O requests at random over the total Addressable Storage Capacity of the TSC for ten (10) minutes at a minimum of 25% of the load used to generate the SPC-1 IOPSTM primary metric. The bit pattern selected to be written to each block as well as the address of the block will be retained in a log file.

The Tested Storage Configuration (TSC) will be shutdown and restarted using a power off/power on cycle at the end of the above sequence of write operations. In addition, any caches employing battery backup must be flushed/emptied.

The SPC-1 Workload Generator will then use the above log file to verify each block written contains the correct bit pattern.

Clause 9.4.3.8

The following content shall appear in this section of the FDR:

1. A listing or screen image of all input parameters supplied to the Workload Generator.
2. For the successful Data Persistence Test Run, a table illustrating key results. The content, appearance, and format of this table are specified in Table 9-12. Information displayed in this table shall be obtained from the Test Run Results File referenced below in #3.
3. For the successful Data Persistence Test Run, the human readable Test Run Results File produced by the Workload Generator.

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 74.

Data Persistence Test Results File

A link to each test result file generated from each Data Persistence Test is listed below.

[Persistence 1 Test Results File](#)

[Persistence 2 Test Results File](#)

Data Persistence Test Results

Data Persistence Test Results	
Data Persistence Test Run Number: 1	
Total Number of Logical Blocks Written	706,167
Total Number of Logical Blocks Verified	703,457
Total Number of Logical Blocks that Failed Verification	0
Time Duration for Writing Test Logical Blocks	5 minutes
Size in Bytes of each Logical Block	1024
Number of Failed I/O Requests in the process of the Test	0

If approved by the SPC Auditor, the SPC-2 Persistence Test may be used to meet the SPC-1 persistence requirements. Both the SPC-1 and SPC-2 Persistence Tests provide the same level of functionality and verification of data integrity. The SPC-2 Persistence Test may be easily configured to address an SPC-1 storage configuration. The SPC-2 Persistence Test extends the size of storage configurations that may be tested and significantly reduces the test duration of such configurations.

The SPC-2 Persistence Test was approved for use in this set of audited measurements.

In some cases the same address was the target of multiple writes, which resulted in more Logical Blocks Written than Logical Blocks Verified. In the case of multiple writes to the same address, the pattern written and verified must be associated with the last write to that address.

PRICED STORAGE CONFIGURATION AVAILABILITY DATE

Clause 9.2.4.9

The committed delivery date for general availability (Availability Date) of all products that comprise the Priced Storage Configuration must be reported. When the Priced Storage Configuration includes products or components with different availability dates, the reported Availability Date for the Priced Storage Configuration must be the date at which all components are committed to be available.

The Huawei OceanStor™ S8100 (4-node) as documented in this Full Disclosure Report is currently available for customer purchase and shipment.

PRICING INFORMATION

Clause 9.4.3.3.6

The Executive Summary shall contain a pricing spreadsheet as documented in Clause 8.3.1.

Pricing information may be found in the Priced Storage Configuration Pricing section on page 14.

TESTED STORAGE CONFIGURATION (TSC) AND PRICED STORAGE CONFIGURATION DIFFERENCES

Clause 9.4.3.3.7

The Executive Summary shall contain a pricing a list of all differences between the Tested Storage Configuration (TSC) and the Priced Storage Configuration.

A list of all differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration may be found in the Executive Summary portion of this document on page 14.

ANOMALIES OR IRREGULARITIES

Clause 9.4.3.10

The FDR shall include a clear and complete description of any anomalies or irregularities encountered in the course of executing the SPC-1 benchmark that may in any way call into question the accuracy, verifiability, or authenticity of information published in this FDR.

There were no anomalies or irregularities encountered during the SPC-1 Remote Audit of the Huawei OceanStor™ S8100 (4-node).

APPENDIX A: SPC-1 GLOSSARY

“Decimal” (*powers of ten*) Measurement Units

In the storage industry, the terms “kilo”, “mega”, “giga”, “tera”, “peta”, and “exa” are commonly used prefixes for computing performance and capacity. For the purposes of the SPC workload definitions, all of the following terms are defined in “powers of ten” measurement units.

- A kilobyte (KB) is equal to 1,000 (10^3) bytes.
- A megabyte (MB) is equal to 1,000,000 (10^6) bytes.
- A gigabyte (GB) is equal to 1,000,000,000 (10^9) bytes.
- A terabyte (TB) is equal to 1,000,000,000,000 (10^{12}) bytes.
- A petabyte (PB) is equal to 1,000,000,000,000,000 (10^{15}) bytes
- An exabyte (EB) is equal to 1,000,000,000,000,000,000 (10^{18}) bytes

“Binary” (*powers of two*) Measurement Units

The sizes reported by many operating system components use “powers of two” measurement units rather than “power of ten” units. The following standardized definitions and terms are also valid and may be used in this document.

- A kibibyte (KiB) is equal to 1,024 (2^{10}) bytes.
- A mebibyte (MiB) is equal to 1,048,576 (2^{20}) bytes.
- A gibibyte (GiB) is equal to 1,073,741,824 (2^{30}) bytes.
- A tebibyte (TiB) is equal to 1,099,511,627,776 (2^{40}) bytes.
- A pebibyte (PiB) is equal to 1,125,899,906,842,624 (2^{50}) bytes.
- An exbibyte (EiB) is equal to 1,152,921,504,606,846,967 (2^{60}) bytes.

SPC-1 Data Repository Definitions

Total ASU Capacity: The total storage capacity read and written in the course of executing the SPC-1 benchmark.

Application Storage Unit (ASU): The logical interface between the storage and SPC-1 Workload Generator. The three ASUs (Data, User, and Log) are typically implemented on one or more Logical Volume.

Logical Volume: The division of Addressable Storage Capacity into individually addressable logical units of storage used in the SPC-1 benchmark. Each Logical Volume is implemented as a single, contiguous address space.

Addressable Storage Capacity: The total storage (sum of Logical Volumes) that can be read and written by application programs such as the SPC-1 Workload Generator.

Configured Storage Capacity: This capacity includes the Addressable Storage Capacity and any other storage (parity disks, hot spares, etc.) necessary to implement the Addressable Storage Capacity.

Physical Storage Capacity: The formatted capacity of all storage devices physically present in the Tested Storage Configuration (TSC).

Data Protection Overhead: The storage capacity required to implement the selected level of data protection.

Required Storage: The amount of Configured Storage Capacity required to implement the Addressable Storage Configuration, excluding the storage required for the three ASUs.

Global Storage Overhead: The amount of Physical Storage Capacity that is required for storage subsystem use and unavailable for use by application programs.

Total Unused Storage: The amount of storage capacity available for use by application programs but not included in the Total ASU Capacity.

SPC-1 Data Protection Levels

Protected: This level will ensure data protection in the event of a single point of failure of any configured storage device. A brief description of the data protection utilized is included in the Executive Summary.

Unprotected: No claim of data protection is asserted in the event of a single point of failure.

SPC-1 Test Execution Definitions

Average Response Time: The sum of the Response Times for all Measured I/O Requests divided by the total number of Measured I/O Requests.

Completed I/O Request: An I/O Request with a Start Time and a Completion Time (see “I/O Completion Types” below).

Completion Time: The time recorded by the Workload Generator when an I/O Request is satisfied by the TSC as signaled by System Software.

Data Rate: The data transferred in all Measured I/O Requests in an SPC-1 Test Run divided by the length of the Test Run in seconds.

Expected I/O Count: For any given I/O Stream and Test Phase, the product of 50 times the BSU level, the duration of the Test Phase in seconds, and the Intensity Multiplier for that I/O Stream.

Failed I/O Request: Any I/O Request issued by the Workload Generator that could not be completed or was signaled as failed by System Software. A Failed I/O Request has no Completion Time (see “I/O Completion Types” below).

I/O Request Throughput: The total number of Measured I/O requests in an SPC-1 Test Run divided by the duration of the Measurement Interval in seconds.

In-Flight I/O Request: An I/O Request issued by the I/O Command Generator to the TSC that has a recorded Start Time, but does not complete within the Measurement Interval (see “I/O Completion Types” below).

Measured I/O Request: A Completed I/O Request with a Completion Time occurring within the Measurement Interval (see “I/O Completion Types” below).

Measured Intensity Multiplier: The percentage of all Measured I/O Requests that were issued by a given I/O Stream.

Measurement Interval: The finite and contiguous time period, after the TSC has reached Steady State, when data is collected by a Test Sponsor to generate an SPC-1 test result or support an SPC-1 test result.

Ramp-Up: The time required for the Benchmark Configuration (BC) to produce Steady State throughput after the Workload Generator begins submitting I/O Requests to the TSC for execution.

Ramp-Down: The time required for the BC to complete all I/O Requests issued by the Workload Generator. The Ramp-Down period begins when the Workload Generator ceases to issue new I/O Requests to the TSC.

Response Time: The Response Time of a Measured I/O Request is its Completion Time minus its Start Time.

Start Time: The time recorded by the Workload Generator when an I/O Request is submitted, by the Workload Generator, to the System Software for execution on the Tested Storage Configuration (TSC).

Start-Up: The period that begins after the Workload Generator starts to submit I/O requests to the TSC and ends at the beginning of the Measurement Interval.

Shut-Down: The period between the end of the Measurement Interval and the time when all I/O Requests issued by the Workload Generator have completed or failed.

Steady State: The consistent and sustainable throughput of the TSC. During this period the load presented to the TSC by the Workload Generator is constant.


Test: A collection of Test Phases and or Test Runs sharing a common objective.

Test Run: The execution of SPC-1 for the purpose of producing or supporting an SPC-1 test result. SPC-1 Test Runs may have a finite and measured Ramp-Up period, Start-Up


period, Shut-Down period, and Ramp-Down period as illustrated in the “SPC-1 Test Run Components” below. All SPC-1 Test Runs shall have a Steady State period and a Measurement Interval.

Test Phase: A collection of one or more SPC-1 Test Runs sharing a common objective and intended to be run in a specific sequence.

I/O Completion Types

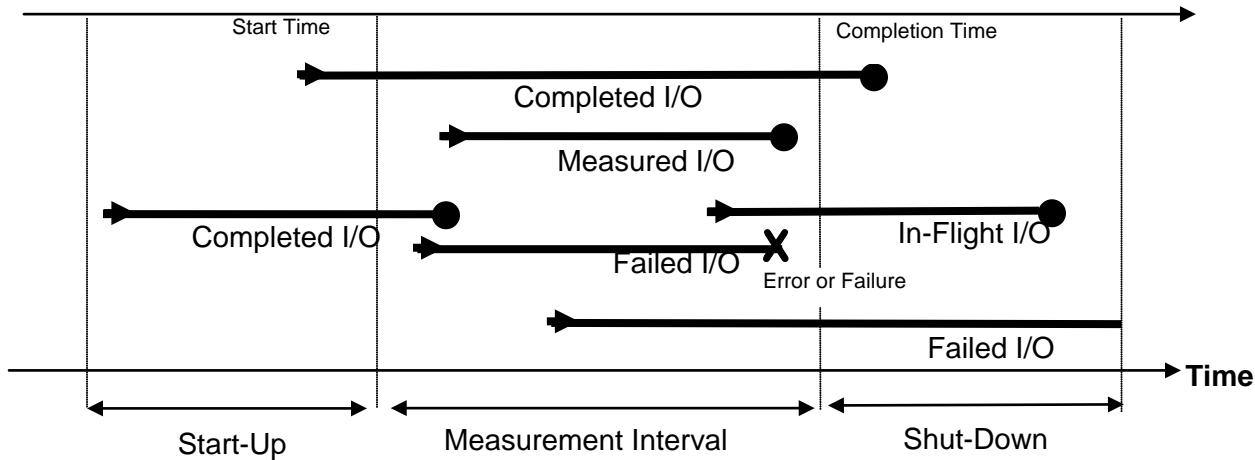

SPC-1 Test Run Components

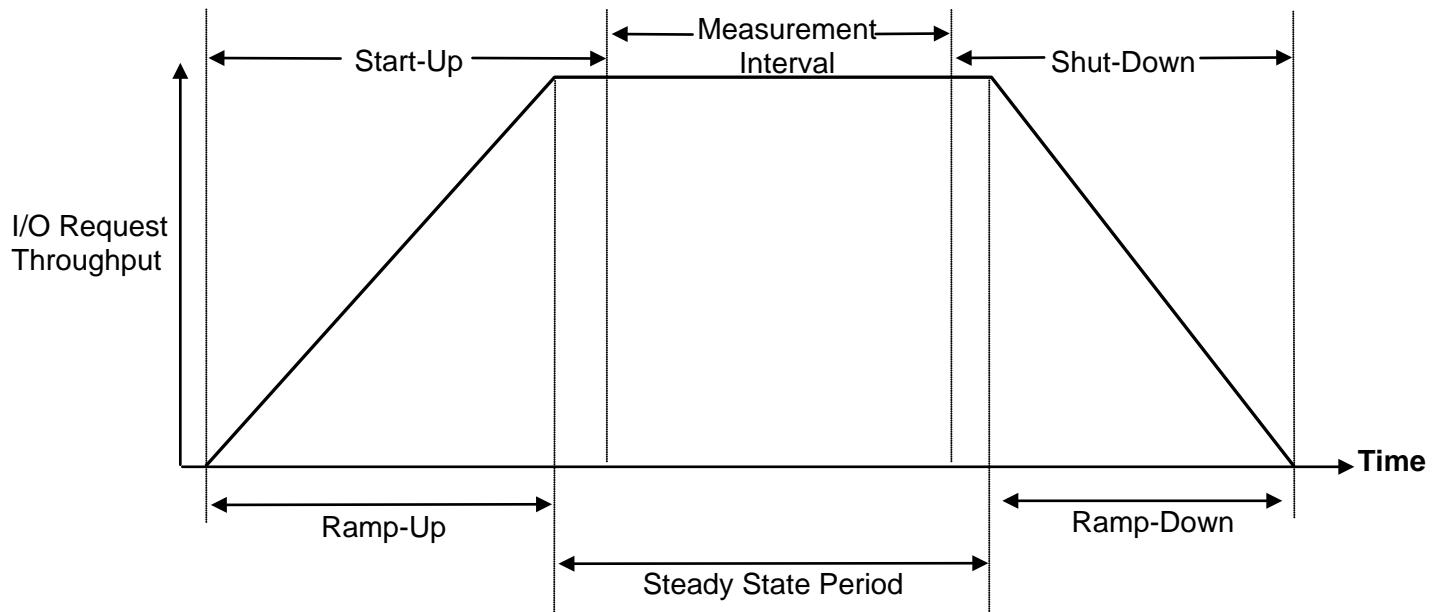

APPENDIX B: CUSTOMER TUNABLE PARAMETERS AND OPTIONS

Windows 2003 Server

The execution throttle, **queue depth**, was changed from a default value of 65535 to 1024 for each HBA in the configuration.

S8100

Enable **write cache with no mirroring**

Set the cache high-low watermarks: **low watermark** is 90% and **high watermark** is 99%

Set the read cache policy to **no prefetch**

APPENDIX C: TESTED STORAGE CONFIGURATION (TSC) CREATION

1. Configure the HBAs

Using **regedit.exe**, change the execution throttle, **queue depth**, in the Windows registry from a default value of 65535 to 1024 for each HBA in the configuration.

2. Create RAID groups and LUNs in the data controller groups

- 2.1 Login to the S8100 CLI console of each of the four data controller groups using SSH, and execute the **raid_lun.script** with the **autobat** S8100 command-line tool. The script will create 12 RAID groups and 24 LUNs (*2 LUNs per RAID group*) in each data controller group. The following is an example to create the RAID groups and LUNs on one data controller group:

OceanStor: admin> autobat -i 129.22.240.65 -u admin -f raid_lun.script

The **createrg** command creates a RAID group. The **createlun** command creates a LUN with a capacity 1,280,000 MiB. The **-p 0** parameter, in the **createlun** command sets the read cache policy as **no prefetch** and the **-m 0** parameter sets the write cache policy as **write cache with no mirroring**.

Each of the LUNs is mapped to a service controller and assigned a unique name, which uses a **sd** prefix. For example, **sdb**, **sdb1**, **sdbx**, and **sddt**.

A listing of **raid_lun.script** appears at the end of this section.

- 2.2 Create two “share” LUNs, each with a capacity of 5,120 MiB, using the S8100 CLI console of one data controller group. Those two LUNs are used for metadata maintenance in the service controller groups. The commands to create the two LUNs are listed below.

OceanStor: admin> createlun -i 0 -n share1 -s 5120 -u 64 -c A -w 1 -m 0

OceanStor: admin> createlun -i 1 -n share2 -s 5120 -u 64 -c A -w 1 -m 0

- 2.3 Login to the S8100 CLI console of each of the four data controller groups using SSH, and change the **high water mark** to **99%** and **low water mark** to **90%** using the following CLI command:

OceanStor: admin> chgcache -h 99 -l 90

raid_lun.script

```
createrg -n RAID10_1 -l 10 -m 2 -d 0,0:0,1:0,2:2,0:2,1:2,2:4,0:4,1:4,2:6,0:6,1:6,2:  
createrg -n RAID10_2 -l 10 -m 2 -d 0,3:0,4:0,5:2,3:2,4:2,5:4,3:4,4:4,5:6,3:6,4:6,5:  
createrg -n RAID10_3 -l 10 -m 2 -d 0,6:0,7:0,8:2,6:2,7:2,8:4,6:4,7:4,8:6,6:6,7:6,8:  
createrg -n RAID10_4 -l 10 -m 2 -d  
0,9:0,10:0,11:2,9:2,10:2,11:4,9:4,10:4,11:6,9:6,10:6,11:  
createrg -n RAID10_5 -l 10 -m 2 -d  
0,12:0,13:0,14:2,12:2,13:2,14:4,12:4,13:4,14:6,12:6,13:6,14:  
createrg -n RAID10_6 -l 10 -m 2 -d  
0,15:0,16:0,17:2,15:2,16:2,17:4,15:4,16:4,17:6,15:6,16:6,17:  
createrg -n RAID10_7 -l 10 -m 2 -d 1,0:1,1:1,2:3,0:3,1:3,2:5,0:5,1:5,2:7,0:7,1:7,2:  
createrg -n RAID10_8 -l 10 -m 2 -d 1,3:1,4:1,5:3,3:3,4:3,5:5,3:5,4:5,5:7,3:7,4:7,5:
```

```

createrg -n RAID10_9 -l 10 -m 2 -d 1,6:1,7:1,8:3,6:3,7:3,8:5,6:5,7:5,8:7,6:7,7:7,8:
createrg -n RAID10_10 -l 10 -m 2 -d
1,9:1,10:1,11:3,9:3,10:3,11:5,9:5,10:5,11:7,9:7,10:7,11:
createrg -n RAID10_11 -l 10 -m 2 -d
1,12:1,13:1,14:3,12:3,13:3,14:5,12:5,13:5,14:7,12:7,13:7,14:
createrg -n RAID10_12 -l 10 -m 2 -d
1,15:1,16:1,17:3,15:3,16:3,17:5,15:5,16:5,17:7,15:7,16:7,17:
createlun -i 0 -n LUN_1 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 0 -n LUN_2 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 1 -n LUN_3 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 1 -n LUN_4 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 2 -n LUN_5 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 2 -n LUN_6 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 3 -n LUN_7 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 3 -n LUN_8 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 4 -n LUN_9 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 4 -n LUN_10 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 5 -n LUN_11 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 5 -n LUN_12 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 6 -n LUN_13 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 6 -n LUN_14 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 7 -n LUN_15 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 7 -n LUN_16 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 8 -n LUN_17 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 8 -n LUN_18 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 9 -n LUN_19 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 9 -n LUN_20 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 10 -n LUN_21 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 10 -n LUN_22 -s 1280000 -u 512 -c A -w 1 -m 0 -p 0
createlun -i 11 -n LUN_23 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0
createlun -i 11 -n LUN_24 -s 1280000 -u 512 -c B -w 1 -m 0 -p 0

```

3. Create disk groups and volumes

- 3.1 Login to the S8100 CLI console of each of the four data controller groups and execute the **www_luns.script** to create a listing of WWN information for each LUN created by **raid_lun.script**. The following is an example to create the listing on one data controller group:

OceanStor: admin> autobat -i 129.22.240.65 -u admin -f www_luns.script

- 3.2 Login to the S8100 CLI console of one of the service controllers and execute the **www_elements.script**, using the command listed below, to create a listing that contains the unique **sd** name and corresponding WWN for each LUN created by **raid_lun.script**.

OceanStor: admin> autobat -i 129.22.240.75 -u admin -f www_elements.script

The information created from **www_luns.script** and **www_elements.script** document the relationship between the LUN names associated with the data controllers and the **sd** names associated with service controllers via the common WWN. This information is used in **disk_volume.script** to create disk groups, each consisting of four LUNs with the same LUN name from the four data controller groups. For example:

- **dg1 (disk group 1)** contains LUNs **sdb**, **sdab**, **sdbx**, **sddt** each identified as **LUN_1** in all four data controller groups.

- **dg2** (*disk group 2*) contains LUNs **sdc**, **sdac**, **sdb**, **sddu** each identified as **LUN_2** in all four data controller groups.
- 3.3 Login to the S8100 CLI console of one of the service controllers and execute the **disk_volume.script** using the command listed below. The script will create 24 disk groups, 24 volumes, and map the 24 volumes to Windows.

OceanStor: admin> autobat -i 129.22.240.75 -u admin -f disk_volume.script

The **vxldg** command creates each disk group in the appropriate service controller group. The **vxassist** command creates each volume in the appropriate service controller group. The entire capacity of each disk group is allocated to each volume, resulting in 24 volumes, each with a capacity of 5,000 GiB (*10,485,760,000 sectors, 512 bytes/sector*).

Listings for **www_luns.script**, **www_elements.script**, and **disk_volume.script** appear below.

www_luns.script

```
showlun -i 0
showlun -i 1
showlun -i 2
showlun -i 3
showlun -i 4
showlun -i 5
showlun -i 6
showlun -i 7
showlun -i 8
showlun -i 9
showlun -i 10
showlun -i 11
showlun -i 12
showlun -i 13
showlun -i 14
showlun -i 15
showlun -i 16
showlun -i 17
showlun -i 18
showlun -i 19
showlun -i 20
showlun -i 21
showlun -i 22
showlun -i 23
```

www_elements.script

```
#!/bin/bash
for i in `vxdisklist |grep 1342.18 |awk '{print $1}'`  
do  
echo $i `vxdisk list $i |grep uid |awk '{print $2}'` | awk -F '%5F' '{print $4}'`  
#vxdisk list $i |grep uid |awk '{print $2}'` | awk -F '%5F' '{print $4}'`  
Done
```

disk_volume.script

```
vxldg -s init dg1 sdb sdab sdbx sddt
vxldg -s init dg2 sdc sdac sdby sddu
vxldg -s init dg3 sdd sdad sdbz sddv
vxldg -s init dg4 sde sdae sdca sddw
```

```
vxdg -s init dg5 sdf sdaf sdcb sddx
vxdg -s init dg6 sdg sdag sdcc sddy
vxdg -s init dg7 sdh sdah sdcd sddz
vxdg -s init dg8 sdi sdai sdce sdea
vxdg -s init dg9 sdj sdaj sdcf sdeb
vxdg -s init dg10 sdk sdak sdcg sdec
vxdg -s init dg11 sdl sdal sdch sded
vxdg -s init dg12 sdm sdam sdci sdee
vxdg -s init dg13 sdn sdan sdcj sdef
vxdg -s init dg14 sdo sdao sdck sdeg
vxdg -s init dg15 sdp sdap sdcl sdeh
vxdg -s init dg16 sdq sdaq sdcm sdei
vxdg -s init dg17 sdr sdar sdcn sdej
vxdg -s init dg18 sds sdas sdco sdek
vxdg -s init dg19 sdt sdat sdcp sdel
vxdg -s init dg20 sdu sdau sdcq sdem
vxdg -s init dg21 sdv sdav sdcr sden
vxdg -s init dg22 sdw sdaw sdcs sdeo
vxdg -s init dg23 sdx sdax sdct sdep
vxdg -s init dg24 sdy sday sdcu sdeq
vxassist -g dg1 make v1 10485760000 layout=stripe sdb sdab sdbx sddt
vxassist -g dg2 make v2 10485760000 layout=stripe sdc sdac sdby sddu
vxassist -g dg3 make v3 10485760000 layout=stripe sdd sdad sdbz sddv
vxassist -g dg4 make v4 10485760000 layout=stripe sde sdae sdca sddw
vxassist -g dg5 make v5 10485760000 layout=stripe sdf sdaf sdcb sddx
vxassist -g dg6 make v6 10485760000 layout=stripe sdg sdag sdcc sddy
vxassist -g dg7 make v7 10485760000 layout=stripe sdh sdah sdcd sddz
vxassist -g dg8 make v8 10485760000 layout=stripe sdi sdai sdce sdea
vxassist -g dg9 make v9 10485760000 layout=stripe sdj sdaj sdcf sdeb
vxassist -g dg10 make v10 10485760000 layout=stripe sdk sdak sdcg sdec
vxassist -g dg11 make v11 10485760000 layout=stripe sdl sdal sdch sded
vxassist -g dg12 make v12 10485760000 layout=stripe sdm sdam sdci sdee
vxassist -g dg13 make v13 10485760000 layout=stripe sdn sdan sdcj sdef
vxassist -g dg14 make v14 10485760000 layout=stripe sdo sdao sdck sdeg
vxassist -g dg15 make v15 10485760000 layout=stripe sdp sdap sdcl sdeh
vxassist -g dg16 make v16 10485760000 layout=stripe sdq sdaq sdcm sdei
vxassist -g dg17 make v17 10485760000 layout=stripe sdr sdar sdcn sdej
vxassist -g dg18 make v18 10485760000 layout=stripe sds sdas sdco sdek
vxassist -g dg19 make v19 10485760000 layout=stripe sdt sdat sdcp sdel
vxassist -g dg20 make v20 10485760000 layout=stripe sdu sdau sdcq sdem
vxassist -g dg21 make v21 10485760000 layout=stripe sdv sdav sdcr sden
vxassist -g dg22 make v22 10485760000 layout=stripe sdw sdaw sdcs sdeo
vxassist -g dg23 make v23 10485760000 layout=stripe sdx sdax sdct sdep
vxassist -g dg24 make v24 10485760000 layout=stripe sdy sday sdcu sdeq
addmap -gi 1 -hl 0 -dg dg1 -v v1
addmap -gi 1 -hl 1 -dg dg2 -v v2
addmap -gi 1 -hl 2 -dg dg3 -v v3
addmap -gi 1 -hl 3 -dg dg4 -v v4
addmap -gi 1 -hl 4 -dg dg5 -v v5
addmap -gi 1 -hl 5 -dg dg6 -v v6
addmap -gi 1 -hl 6 -dg dg7 -v v7
addmap -gi 1 -hl 7 -dg dg8 -v v8
addmap -gi 1 -hl 8 -dg dg9 -v v9
addmap -gi 1 -hl 9 -dg dg10 -v v10
addmap -gi 1 -hl 10 -dg dg11 -v v11
addmap -gi 1 -hl 11 -dg dg12 -v v12
addmap -gi 1 -hl 12 -dg dg13 -v v13
addmap -gi 1 -hl 13 -dg dg14 -v v14
addmap -gi 1 -hl 14 -dg dg15 -v v15
addmap -gi 1 -hl 15 -dg dg16 -v v16
addmap -gi 1 -hl 16 -dg dg17 -v v17
addmap -gi 1 -hl 17 -dg dg18 -v v18
addmap -gi 1 -hl 18 -dg dg19 -v v19
```

```
addmap -gi 1 -hl 19 -dg dg20 -v v20
addmap -gi 1 -hl 20 -dg dg21 -v v21
addmap -gi 1 -hl 21 -dg dg22 -v v22
addmap -gi 1 -hl 22 -dg dg23 -v v23
addmap -gi 1 -hl 23 -dg dg24 -v v24
```

4. Create Windows stripe volumes

The **doSPC.bat** script is executed from a command line window on the Host System and invokes the Windows Diskpart utility to perform the following:

- Convert disk type for MBR to GPT using **convertGPT.script**
- Convert all Basic disks to Dynamic disks using **convertDynamic.script**
- Complete the following steps using **createVolumes.script**:
 - Create one unformatted, striped (RAID 0) volume, without an assigned drive letter, using 32 MiB of each of the 24 Dynamic disks.
 - Create twenty unformatted, striped (RAID 0) volumes, using 196,608 MiB of each of the 24 Dynamic disks and assign drive letters “F” to “Y” to the volumes. The twenty volumes comprise the SPC-1 Logical Volumes.

doSPC.bat

```
@echo ****
@echo * Warning make sure your boot device is PhysicalDrive 0 *
@echo ****

timeout /t 15 /NOBREAK
diskpart /s convertGPT.script
timeout /t 15 /NOBREAK
diskpart /s convertDynamic.script
timeout /t 15 /NOBREAK
diskpart /s createVolumes.script
```

convertGPT.script

```
select disk 1
convert gpt noerr
select disk 2
convert gpt noerr
select disk 3
convert gpt noerr
select disk 4
convert gpt noerr
select disk 5
convert gpt noerr
select disk 6
convert gpt noerr
select disk 7
convert gpt noerr
select disk 8
convert gpt noerr
select disk 9
convert gpt noerr
select disk 10
convert gpt noerr
```

```
select disk 11
convert gpt noerr
select disk 12
convert gpt noerr
select disk 13
convert gpt noerr
select disk 14
convert gpt noerr
select disk 15
convert gpt noerr
select disk 16
convert gpt noerr
select disk 17
convert gpt noerr
select disk 18
convert gpt noerr
select disk 19
convert gpt noerr
select disk 20
convert gpt noerr
select disk 21
convert gpt noerr
select disk 22
convert gpt noerr
select disk 23
convert gpt noerr
select disk 24
convert gpt noerr
```

convertDynamic.script

```
select disk 1
convert dynamic noerr
select disk 2
convert dynamic noerr
select disk 3
convert dynamic noerr
select disk 4
convert dynamic noerr
select disk 5
convert dynamic noerr
select disk 6
convert dynamic noerr
select disk 7
convert dynamic noerr
select disk 8
convert dynamic noerr
select disk 9
convert dynamic noerr
select disk 10
convert dynamic noerr
select disk 11
convert dynamic noerr
select disk 12
convert dynamic noerr
select disk 13
convert dynamic noerr
select disk 14
convert dynamic noerr
select disk 15
convert dynamic noerr
select disk 16
```

```
convert dynamic noerr
select disk 17
convert dynamic noerr
select disk 18
convert dynamic noerr
select disk 19
convert dynamic noerr
select disk 20
convert dynamic noerr
select disk 21
convert dynamic noerr
select disk 22
convert dynamic noerr
select disk 23
convert dynamic noerr
select disk 24
convert dynamic noerr
```

createVolumes.script

```
create volume stripe size=32
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=F
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=G
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=H
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=I
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=J
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=K
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=L
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=M
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=N
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=O
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=P
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=Q
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=R
```

```
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=S
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=T
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=U
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=V
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=W
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=X
create volume stripe size=196608
disk=1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24
assign letter=Y
```

APPENDIX D: SPC-1 WORKLOAD GENERATOR STORAGE COMMANDS AND PARAMETERS

The content of SPC-1 Workload Generator command and parameter file, used in this benchmark to execute the Primary Metrics and Repeatability Tests, is listed below.

```
javaparms="-Xmx3000m -Xms1200m -Xss256k"
sd=asul_1,lun=\.\F:,size=4608g
sd=asul_2,lun=\.\G:,size=4608g
sd=asul_3,lun=\.\H:,size=4608g
sd=asul_4,lun=\.\I:,size=4608g
sd=asul_5,lun=\.\J:,size=4608g
sd=asul_6,lun=\.\K:,size=4608g
sd=asul_7,lun=\.\L:,size=4608g
sd=asul_8,lun=\.\M:,size=4608g
sd=asul_9,lun=\.\N:,size=4608g
sd=asu2_1,lun=\.\O:,size=4608g
sd=asu2_2,lun=\.\P:,size=4608g
sd=asu2_3,lun=\.\Q:,size=4608g
sd=asu2_4,lun=\.\R:,size=4608g
sd=asu2_5,lun=\.\S:,size=4608g
sd=asu2_6,lun=\.\T:,size=4608g
sd=asu2_7,lun=\.\U:,size=4608g
sd=asu2_8,lun=\.\V:,size=4608g
sd=asu2_9,lun=\.\W:,size=4608g
sd=asu3_1,lun=\.\X:,size=4608g
sd=asu3_2,lun=\.\Y:,size=4608g
```

The content of SPC-2 Workload Generator command and parameter file, used in this benchmark to execute the Persistence Test, is listed below.

Persistence Test Run 1 (write phase)

```
host=localhost,jvms=4,maxstreams=200
sd=sd1,lun=\.\F:,size=4608g
sd=sd2,lun=\.\G:,size=4608g
sd=sd3,lun=\.\H:,size=4608g
sd=sd4,lun=\.\I:,size=4608g
sd=sd5,lun=\.\J:,size=4608g
sd=sd6,lun=\.\K:,size=4608g
sd=sd7,lun=\.\L:,size=4608g
sd=sd8,lun=\.\M:,size=4608g
sd=sd9,lun=\.\N:,size=4608g
sd=sd10,lun=\.\O:,size=4608g
sd=sd11,lun=\.\P:,size=4608g
sd=sd12,lun=\.\Q:,size=4608g
sd=sd13,lun=\.\R:,size=4608g
sd=sd14,lun=\.\S:,size=4608g
sd=sd15,lun=\.\T:,size=4608g
sd=sd16,lun=\.\U:,size=4608g
sd=sd17,lun=\.\V:,size=4608g
sd=sd18,lun=\.\W:,size=4608g
sd=sd19,lun=\.\X:,size=4608g
sd=sd20,lun=\.\Y:,size=4608g
maxlatetestart=1
reportinginterval=5
segmentlength=512m
rd=default,rampup=180,periods=90,measurement=300,runout=0,rampdown=0,buffers=1
rd=default,rdpct=0,xfersize=1024k
rd=TR1-124s_SPC-2-persist-w,streams=124
```

Persistence Test Run 2 (read phase)

```
host=localhost,jvms=4,maxstreams=200
sd=sd1,lun=\.\F:,size=4608g
sd=sd2,lun=\.\G:,size=4608g
sd=sd3,lun=\.\H:,size=4608g
sd=sd4,lun=\.\I:,size=4608g
sd=sd5,lun=\.\J:,size=4608g
sd=sd6,lun=\.\K:,size=4608g
sd=sd7,lun=\.\L:,size=4608g
sd=sd8,lun=\.\M:,size=4608g
sd=sd9,lun=\.\N:,size=4608g
sd=sd10,lun=\.\O:,size=4608g
sd=sd11,lun=\.\P:,size=4608g
sd=sd12,lun=\.\Q:,size=4608g
sd=sd13,lun=\.\R:,size=4608g
sd=sd14,lun=\.\S:,size=4608g
sd=sd15,lun=\.\T:,size=4608g
sd=sd16,lun=\.\U:,size=4608g
sd=sd17,lun=\.\V:,size=4608g
sd=sd18,lun=\.\W:,size=4608g
sd=sd19,lun=\.\X:,size=4608g
sd=sd20,lun=\.\Y:,size=4608g
maxlateteststart=1
reportinginterval=5
segmentlength=512m
maxpersistenceerrors=10
rd=default,buffers=1,rdpct=100,xfersize=1024k
rd=TR1-124s_SPC-2-persist-r
```

APPENDIX E: SPC-1 WORKLOAD GENERATOR INPUT PARAMETERS

Primary Metrics Test, Repeatability Test, and Persistence Test Run 1

The following script was used to execute the Primary Metrics Test (*Sustainability Test Phase, IOPS Test Phase, and Response Time Ramp Test Phase*), Repeatability Test (*Repeatability Test Phase 1 and Repeatability Test Phase 2*), and Persistence Test Run 1 in an uninterrupted sequence.

```
@echo off
echo list volume >> volume.script
for /l %%i in (1 1 20) do (
    echo select volume %%i >> volume.script
    echo detail volume >>volume.script
)
diskpart /s volume.script >>partitionedhostsystem.txt
cd "c:\spc\spc1"
java -Xmx3000m -Xms2048m metrics -b 3201
java -Xmx3000m -Xms2048m repeat1 -b 3201
java -Xmx3000m -Xms2048m repeat2 -b 3201
cd "c:\spc\spc2"
call spc2.bat -f persist1.cfg -o init -init
call spc2.bat -f persist1.cfg -o persist1
```

Persistence Test Run 2

The following script was used to execute Persistence Test Run 2.

```
@echo off
echo list volume >> volume.persist2.script
for /l %%i in (1 1 20) do (
    echo select volume %%i >> volume.persist2.script
    echo detail volume >>volume.persist2.script
)
diskpart /s volume.persist2.script >>partitionedhostsystemofpersist2.txt
cd "c:\spc\spc2"
call spc2.bat -f persist2.cfg -o persist2
```