



SPC BENCHMARK 1™
FULL DISCLOSURE REPORT

HUAWEI TECHNOLOGIES Co., LTD.
HUAWEI OCEANSTOR™ S5800T

SPC-1 V1.13

Submitted for Review: November 15, 2012
Submission Identifier: A00124

First Edition – November 2012

THE INFORMATION CONTAINED IN THIS DOCUMENT IS DISTRIBUTED ON AN AS IS BASIS WITHOUT ANY WARRANTY EITHER EXPRESS OR IMPLIED. The use of this information or the implementation of any of these techniques is the customer's responsibility and depends on the customer's ability to evaluate and integrate them into the customer's operational environment. While each item has been reviewed by Huawei Technologies Co., Ltd. for accuracy in a specific situation, there is no guarantee that the same or similar results will be obtained elsewhere. Customers attempting to adapt these techniques to their own environment do so at their own risk.

This publication was produced in the United States. Huawei Technologies Co., Ltd. may not offer the products, services, or features discussed in this document in other countries, and the information is subject to change with notice. Consult your local Huawei Technologies Co., Ltd. representative for information on products and services available in your area.

© Copyright Huawei Technologies Co., Ltd. 2012. All rights reserved.

Permission is hereby granted to reproduce this document in whole or in part, provided the copyright notice as printed above is set forth in full text on the title page of each item reproduced.

Trademarks

SPC Benchmark-1, SPC-1, SPC-1 IOPS, SPC-1 LRT and SPC-1 Price-Performance are trademarks of the Storage Performance Council. Huawei, the Huawei logo and OceanStor are trademarks or registered trademarks of Huawei Technologies Co., Ltd. in the United States and other countries. All other brands, trademarks, and product names are the property of their respective owners.

Table of Contents

Audit Certification.....	vii
Audit Certification (<i>cont.</i>)	viii
Letter of Good Faith	ix
Executive Summary.....	10
Test Sponsor and Contact Information.....	10
Revision Information and Key Dates	10
Tested Storage Product (TSP) Description.....	10
Summary of Results	11
Storage Capacities, Relationships, and Utilization	12
Response Time – Throughput Curve	13
Response Time – Throughput Data.....	13
Differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration.....	14
Priced Storage Configuration Pricing	14
Priced Storage Configuration Diagram.....	16
Priced Storage Configuration Components.....	16
Configuration Information	17
Benchmark Configuration (BC)/Tested Storage Configuration (TSC) Diagram.	17
Storage Network Configuration	17
Host System(s) and Tested Storage Configuration (TSC) Table of Components	17
Benchmark Configuration/Tested Storage Configuration Diagram.....	18
Host Systems and Tested Storage Configuration Components.....	18
Customer Tunable Parameters and Options	19
Tested Storage Configuration (TSC) Description	19
SPC-1 Workload Generator Storage Configuration	19
ASU Pre-Fill.....	20
SPC-1 Data Repository.....	21
Storage Capacities and Relationships	21
SPC-1 Storage Capacities	21
SPC-1 Storage Capacities and Relationships Illustration.....	22
SPC-1 Storage Hierarchy Ratios	22
Storage Capacity Utilization	23
Logical Volume Capacity and ASU Mapping	23
SPC-1 Benchmark Execution Results.....	24
SPC-1 Tests, Test Phases, and Test Runs.....	24

Primary Metrics Test – Sustainability Test Phase	26
SPC-1 Workload Generator Input Parameters	26
Sustainability Test Results File	26
Sustainability – Data Rate Distribution Data (<i>MB/second</i>)	27
Sustainability – Data Rate Distribution Graph	27
Sustainability – I/O Request Throughput Distribution Data	28
Sustainability – I/O Request Throughput Distribution Graph	28
Sustainability – Average Response Time (ms) Distribution Data	29
Sustainability – Average Response Time (ms) Distribution Graph	29
Sustainability – Response Time Frequency Distribution Data	30
Sustainability – Response Time Frequency Distribution Graph	30
Sustainability – Measured Intensity Multiplier and Coefficient of Variation.....	31
Primary Metrics Test – IOPS Test Phase.....	32
SPC-1 Workload Generator Input Parameters	32
IOPS Test Results File.....	32
IOPS Test Run – I/O Request Throughput Distribution Data	33
IOPS Test Run – I/O Request Throughput Distribution Graph.....	33
IOPS Test Run – Average Response Time (ms) Distribution Data	34
IOPS Test Run – Average Response Time (ms) Distribution Graph	34
IOPS Test Run – Response Time Frequency Distribution Data	35
IOPS Test Run –Response Time Frequency Distribution Graph.....	35
IOPS Test Run – I/O Request Information	36
IOPS Test Run – Measured Intensity Multiplier and Coefficient of Variation	36
Primary Metrics Test – Response Time Ramp Test Phase	37
SPC-1 Workload Generator Input Parameters	37
Response Time Ramp Test Results File.....	37
Response Time Ramp Distribution (IOPS) Data	38
Response Time Ramp Distribution (IOPS) Graph	39
SPC-1 LRT™ Average Response Time (ms) Distribution Data.....	40
SPC-1 LRT™ Average Response Time (ms) Distribution Graph	40
SPC-1 LRT™ (10%) – Measured Intensity Multiplier and Coefficient of Variation	41
Repeatability Test	42
SPC-1 Workload Generator Input Parameters	42
Repeatability Test Results File	43
Repeatability 1 LRT – I/O Request Throughput Distribution Data.....	44
Repeatability 1 LRT – I/O Request Throughput Distribution Graph	44
Repeatability 1 LRT –Average Response Time (ms) Distribution Data	45
Repeatability 1 LRT –Average Response Time (ms) Distribution Graph	45
Repeatability 1 IOPS – I/O Request Throughput Distribution Data	46

Repeatability 1 IOPS – I/O Request Throughput Distribution Graph.....	46
Repeatability 1 IOPS –Average Response Time (ms) Distribution Data	47
Repeatability 1 IOPS –Average Response Time (ms) Distribution Graph	47
Repeatability 2 LRT – I/O Request Throughput Distribution Data.....	48
Repeatability 2 LRT – I/O Request Throughput Distribution Graph	48
Repeatability 2 LRT –Average Response Time (ms) Distribution Data	49
Repeatability 2 LRT –Average Response Time (ms) Distribution Graph.....	49
Repeatability 2 IOPS – I/O Request Throughput Distribution Data	50
Repeatability 2 IOPS – I/O Request Throughput Distribution Graph.....	50
Repeatability 2 IOPS –Average Response Time (ms) Distribution Data.....	51
Repeatability 2 IOPS –Average Response Time (ms) Distribution Graph	51
Repeatability 1 (LRT) Measured Intensity Multiplier and Coefficient of Variation	52
Repeatability 1 (IOPS) Measured Intensity Multiplier and Coefficient of Variation	52
Repeatability 2 (LRT) Measured Intensity Multiplier and Coefficient of Variation	52
Repeatability 2 (IOPS) Measured Intensity Multiplier and Coefficient of Variation	53
Data Persistence Test.....	54
SPC-1 Workload Generator Input Parameters	54
Data Persistence Test Results File	54
Data Persistence Test Results.....	55
Priced Storage Configuration Availability Date.....	56
Pricing Information.....	56
Tested Storage Configuration (TSC) and Priced Storage Configuration Differences.....	56
Anomalies or Irregularities	56
Appendix A: SPC-1 Glossary	57
“Decimal” (<i>powers of ten</i>) Measurement Units	57
“Binary” (<i>powers of two</i>) Measurement Units.....	57
SPC-1 Data Repository Definitions.....	57
SPC-1 Data Protection Levels	58
SPC-1 Test Execution Definitions	58
I/O Completion Types	60
SPC-1 Test Run Components.....	60
Appendix B: Customer Tunable Parameters and Options.....	61
Red Hat Enterprise Linux 5.5 (64-bit)	61
Appendix C: Tested Storage Configuration (TSC) Creation	62
Step 1 Create Host Group and Host.....	62
Step 2 Create RAID Groups and LUNs.....	62

Step 3 Change the low and high water level of storage	63
Step 4 Create Volumes on the Host System	63
1. Create Physical Volumes	63
2. Create Volume Groups.....	64
3. Create Logical Volumes	64
4. Scan Logical Volumes	64
Step 5 Change the schedule on each block device	64
Referenced Scripts.....	64
mklun.sh	64
mkvolume.sh	66
scheduler.sh.....	68
Appendix D: SPC-1 Workload Generator Storage Commands and Parameters	69
ASU Pre-Fill.....	69
Primary Metrics and Repeatability Tests	70
SPC-1 Persistence Test.....	71
Appendix E: SPC-1 Workload Generator Input Parameters	72
ASU Pre-Fill, Primary Metrics Test, Repeatability Test, Persistence Test Run 1, TSC power off/power on and Persistence Test Run 2.....	72
Appendix F: Third-Party Quotation.....	75

AUDIT CERTIFICATION



Gradient
SYSTEMS

Eric He
 Huawei Technologies Co., Ltd.
 Tianchen Road 88#
 Chengdu, Sichuan, P.R. China 611711

November 13, 2012

The SPC Benchmark 1™ Reported Data listed below for the Huawei OceanStor™ S5800T was produced in compliance with the SPC Benchmark 1™ v1.13 Remote Audit requirements.

SPC Benchmark 1™ v1.13 Reported Data	
Tested Storage Product (TSP) Name:	
Metric	Reported Result
SPC-1 IOPS™	150,286.25
SPC-1 Price-Performance	\$3.16/SPC-1 IOPS™
Total ASU Capacity	50,465.866 GB
Data Protection Level	Protected (<i>Mirroring</i>)
Total TSC Price (including three-year maintenance)	\$475,090.00

The following SPC Benchmark 1™ Remote Audit requirements were reviewed and found compliant with 1.13 of the SPC Benchmark 1™ specification:

- A Letter of Good Faith, signed by a senior executive.
- The following Data Repository storage items were verified by information supplied by Huawei Technologies Co., Ltd:
 - ✓ Physical Storage Capacity and requirements.
 - ✓ Configured Storage Capacity and requirements.
 - ✓ Addressable Storage Capacity and requirements.
 - ✓ Capacity of each Logical Volume and requirements.
 - ✓ Capacity of each Application Storage Unit (ASU) and requirements.
- The total Application Storage Unit (ASU) Capacity was filled with random data, using an auditor approved tool, prior to execution of the SPC-1 Tests.
- An appropriate diagram of the Benchmark Configuration (BC)/Tested Storage Configuration (TSC).

Storage Performance Council
 643 Bair Island Road, Suite 103
 Redwood City, CA 94062
AuditService@storageperformance.org
 650.556.9384

AUDIT CERTIFICATION (CONT.)

Huawei OceanStor™ S5800T
SPC-1 Audit Certification

Page 2

- Listings and commands to configure the Benchmark Configuration/Tested Storage Configuration, including customer tunable parameters that were changed from default values.
- SPC-1 Workload Generator commands and parameters used for the audited SPC Test Runs.
- The following Host System requirements were verified by information supplied by Huawei Technologies Co., Ltd.:
 - ✓ The type of each Host System including the number of processors and main memory.
 - ✓ The presence and version number of the SPC-1 Workload Generator on each Host System.
 - ✓ The TSC boundary within each Host System.
- The Test Results Files and resultant Summary Results Files received from Huawei Technologies Co., Ltd. for each of following were authentic, accurate, and compliant with all of the requirements and constraints of Clauses 4 and 5 of the SPC-1 Benchmark Specification:
 - ✓ Data Persistence Test
 - ✓ Sustainability Test Phase
 - ✓ IOPS Test Phase
 - ✓ Response Time Ramp Test Phase
 - ✓ Repeatability Test
- There were no differences between the Tested Storage Configuration and Priced Storage Configuration.
- The submitted pricing information met all of the requirements and constraints of Clause 8 of the SPC-1 Benchmark Specification.
- The Full Disclosure Report (FDR) met all of the requirements in Clause 9 of the SPC-1 Benchmark Specification.
- This successfully audited SPC measurement is not subject to an SPC Confidential Review.

Audit Notes:

There were no audit notes or exceptions.

Respectfully,

Walter E. Baker
SPC Auditor

Storage Performance Council
643 Bair Island Road, Suite 103
Redwood City, CA 94062
AuditService@storageperformance.org
650.556.9384

LETTER OF GOOD FAITH



©Huawei Technologies Co., Ltd.

Huawei Industrial Base, Bantian, Longgang

Shenzhen city

Guangdong province

China

Tel: 0086-755-28780808

<http://www.huawei.com/en/>

Date: November 7, 2012

From: Huawei Technologies Co., Ltd.


To: Walter E. Baker, SPC Auditor
Gradient Systems, Inc.
643 Bair Island Road, Suite 103
Redwood City, CA 94063

Subject: SPC-1 Letter of Good Faith for the Huawei OceanStor S5800T

Huawei Technologies Co., Ltd. is the SPC-1 Test Sponsor for the above listed product. To the best of our knowledge and belief, the required SPC-1 benchmark results and materials we have submitted for that product are complete, accurate, and in full compliance with V1.13 of the SPC-1 benchmark specification.


In addition, we have reported any items in the Benchmark Configuration and execution of the benchmark that affected the reported results even if the items are not explicitly required to be disclosed by the SPC-1 benchmark specification.

Signed:



Fan Ruiqi
President of Storage Product Line

Date:



2012.11.7

EXECUTIVE SUMMARY

Test Sponsor and Contact Information

Test Sponsor and Contact Information	
Test Sponsor Primary Contact	Huawei Technologies Co., Ltd. – http://www.huawei.com/en/ Eric He – eric.heji@huawei.com Tianchen Road 88# Chengdu, Sichuan, P.R. China 611711 Phone: 86 28 62905595 FAX: 86 28 62905793
Test Sponsor Alternate Contact	Huawei Technologies Co., Ltd. – http://www.huawei.com/en/ Xu Zhong – xuzhong@huawei.com Tianchen Road 88# Chengdu, Sichuan, P.R. China 611711 Phone: 86 28 62905591 FAX: 86 28 62905793
Auditor	Storage Performance Council – http://www.storageperformance.org Walter E. Baker – AuditService@StoragePerformance.org 643 Bair Island Road, Suite 103 Redwood City, CA 94063 Phone: (650) 556-9384 FAX: (650) 556-9385

Revision Information and Key Dates

Revision Information and Key Dates	
SPC-1 Specification revision number	V1.13
SPC-1 Workload Generator revision number	V2.3.0
Date Results were first used publicly	November 15, 2012
Date the FDR was submitted to the SPC	November 15, 2012
Date the Priced Storage Configuration is available for shipment to customers	currently available
Date the TSC completed audit certification	November 13, 2012

Tested Storage Product (TSP) Description

Huawei OceanStor T series unified storage system (T series) is a new-generation storage product for mid-range and high-end storage applications. It boasts integration of block-level and file-level data storage, support for a variety of storage protocols, and GUI-based central storage management. Delivering leading performance, enhanced efficiency, maximized return on investment, and all-in-one solutions, the T series is ideally applicable to scenarios such as large-database OLTP/OLAP, high-performance computing, digital media, Internet applications, central storage, backup, disaster recovery, and data migration.

Summary of Results

SPC-1 Reported Data	
Tested Storage Product (TSP) Name: Huawei OceanStor™ S5800T	
Metric	Reported Result
SPC-1 IOPS™	150,286.25
SPC-1 Price-Performance™	\$3.16/SPC-1 IOPS™
Total ASU Capacity	50,465.866 GB
Data Protection Level	Protected 1 (<i>Mirroring</i>)
Total Price	\$475,090.00
Currency Used	U.S. Dollars
Target Country for availability, sales and support	USA

SPC-1 IOPS™ represents the maximum I/O Request Throughput at the 100% load point.

SPC-1 Price-Performance™ is the ratio of **Total Price** to **SPC-1 IOPS™**.

Total ASU (Application Storage Unit) Capacity represents the total storage capacity available to be read and written in the course of executing the SPC-1 benchmark.

A **Data Protection Level** of [Protected 1](#) using *Mirroring* configures two or more identical copies of user data.


Total Price includes the cost of the Priced Storage Configuration plus three years of hardware maintenance and software support as detailed on page 14.

Currency Used is formal name for the currency used in calculating the **Total Price** and **SPC-1 Price-Performance™**. That currency may be the local currency of the **Target Country** or the currency of a difference country (*non-local currency*).

The **Target Country** is the country in which the Priced Storage Configuration is available for sale and in which the required hardware maintenance and software support is provided either directly from the Test Sponsor or indirectly via a third-party supplier.

Storage Capacities, Relationships, and Utilization

The following diagram (*not to scale*) and table document the various storage capacities, used in this benchmark, and their relationships, as well as the storage utilization values required to be reported.

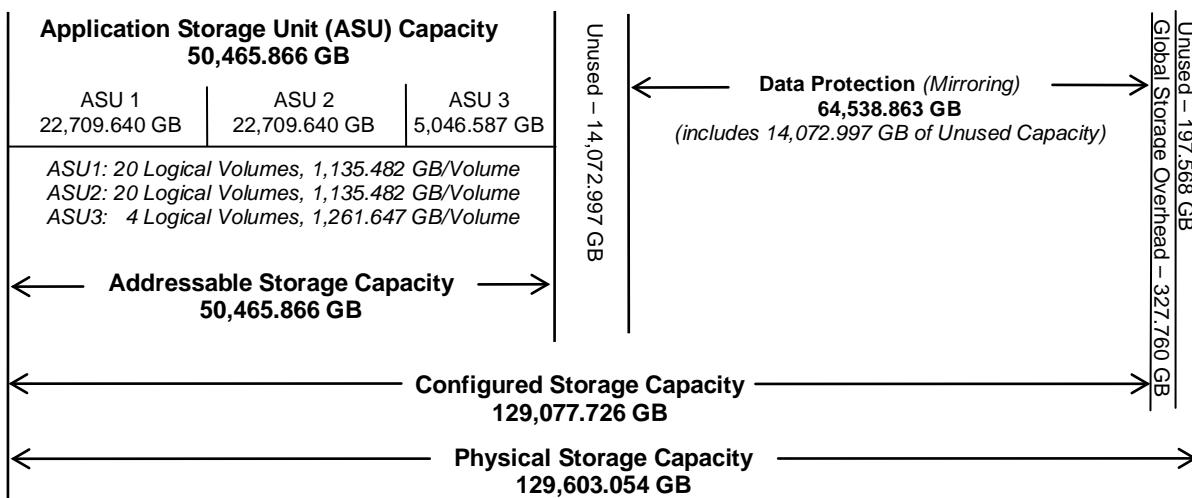

SPC-1 Storage Capacity Utilization	
Application Utilization	38.94%
Protected Application Utilization	77.88%
Unused Storage Ratio	21.87%

Application Utilization: Total ASU Capacity (**50,465.866 GB**) divided by Physical Storage Capacity (**129,603.054 GB**)

Protected Application Utilization: Total ASU Capacity (**50,465.866 GB**) plus total Data Protection Capacity (**64,538.863 GB**) minus unused Data Protection Capacity (**14,072.997 GB**) divided by Physical Storage Capacity (**129,603.054 GB**)


Unused Storage Ratio: Total Unused Capacity (**28,343.563 GB**) divided by Physical Storage Capacity (**129,603.054 GB**) and may not exceed 45%.

Detailed information for the various storage capacities and utilizations is available on pages 21-22.

Response Time – Throughput Curve

The Response Time-Throughput Curve illustrates the Average Response Time (milliseconds) and I/O Request Throughput at 100%, 95%, 90%, 80%, 50%, and 10% of the workload level used to generate the SPC-1 IOPS™ metric.

The Average Response Time measured at any of the above load points cannot exceed 30 milliseconds or the benchmark measurement is invalid.

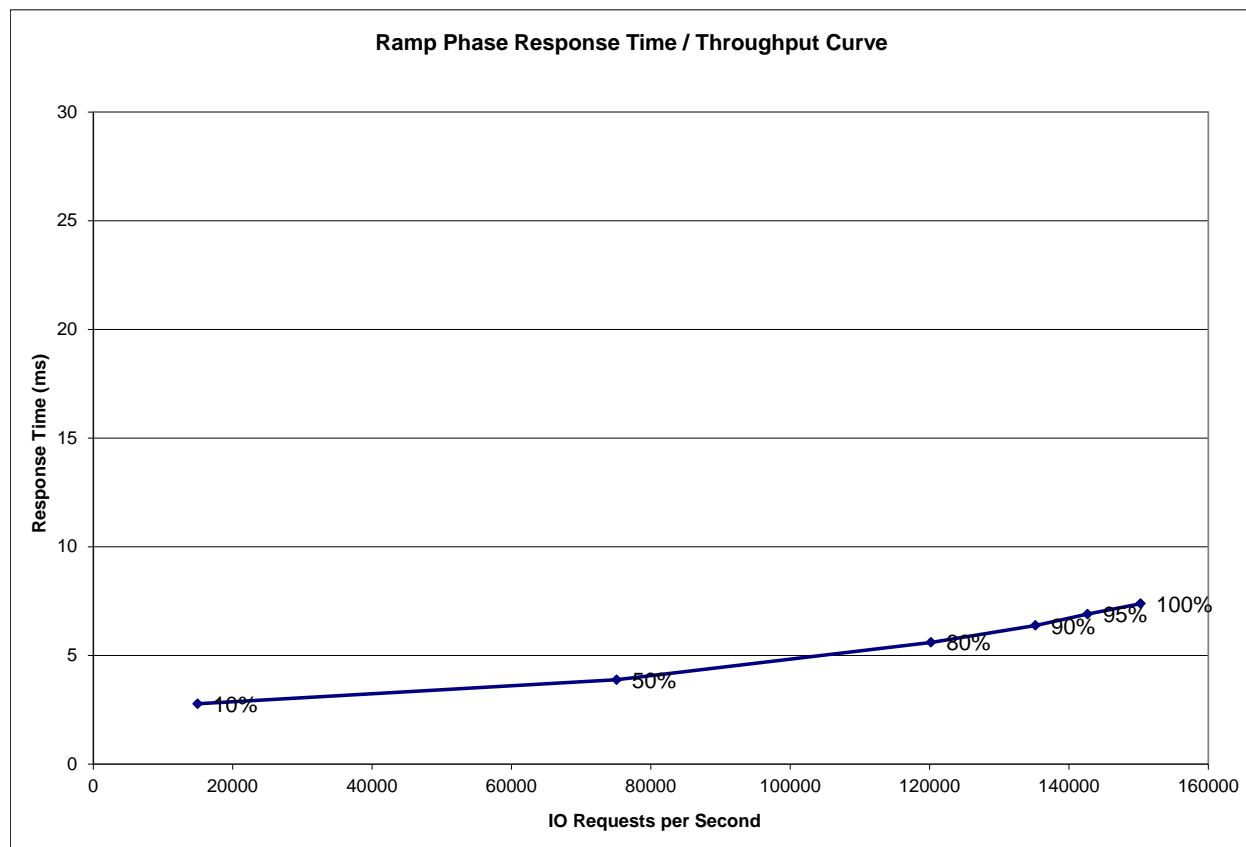

Response Time – Throughput Data

	10% Load	50% Load	80% Load	90% Load	95% Load	100% Load
I/O Request Throughput	14,994.14	75,086.00	120,196.06	135,195.89	142,677.38	150,286.25
Average Response Time (ms):						
All ASUs	2.77	3.88	5.60	6.38	6.90	7.38
ASU-1	3.67	5.02	7.03	7.94	8.51	9.03
ASU-2	3.30	5.31	8.47	10.06	11.14	12.29
ASU-3	0.62	0.83	1.31	1.45	1.63	1.73
Reads	6.21	8.68	12.32	14.07	15.13	16.21
Writes	0.53	0.75	1.22	1.36	1.54	1.63

Differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration

There were no differences between the TSC and Priced Storage Configuration.

Priced Storage Configuration Pricing


Part Number	Description	Quantity	Unit Price	Total Price
Control module				43,757.00
SPE61C0200-S56-2C96G-BASE	SPE61C0200-56 Controller Enclosure(Dual Controller,AC,96GB Cache,with UPS Cache Protected Module,without Front-End & Back-End Port,with HS Storage Array Control System Software)	1	43,757.00	43,757.00
Hard Disk Drives				176,568.00
SAS300-15K-2	300GB 15K RPM SAS Disk Unit(3.5")	384	418.00	160,512.00
SAS600-15K-2	600GB 15K RPM SAS Disk Unit(3.5")	24	669.00	16,056.00
Disk Enclosure				51,102.00
DAE12435U4-AC	DAE12435U4-03 Disk Enclosure(4U,3.5",AC,SAS Expansion Module,without Disk Unit,with HS SAS in Band Management Software)	17	3,006.00	51,102.00
IO Interface				10,710.00
LPU4F8	4*8Gbps Fibre Channel I/O modules(Total 4 ports)	2	1,219.00	2,438.00
LPU2S6	2*24Gbps SAS-wide I/O modules(Total 2 ports)	8	1,034.00	8,272.00
Accessory				519.00
SS-OP-D-LC-M-3	Patchcord,DLC/PC-DLC/PC,Multimode,2mm Parallel,3m	8	11.00	88.00
MINI-SAS-3	Purchased Cable,MiniSAS Cable,Key246,3m	1	67.00	67.00
MINI-SAS-6	Purchased Cable,MiniSAS Cable,Key246,3m	4	91.00	364.00
Storage management software				6,074.00
LIC-UltraPath02-V1R5	OceanStor HS UltraPath Software License	1	1,938.00	1,938.00
LIC-S5B-ISM02-BLOCK	HS Integrated Storage Manager-Device Management License for OceanStor Block S5800T	1	4,136.00	4,136.00
Third Party				6,792.00
N8GHBA000	QLOGIC QLE2562 HBA Card,PCIe,8Gbps DualPort ,Fiber Channel Multimode LC Optic Interface,English Manual,Driver CD	4	1,698.00	6,792.00
Total of Product				295,522.00
Maintenance Support Service				179,568.00
Hi-Care Premier On-Site Service (3 years)		1	179,568.00	179,568.00
Total of Service (3 years)				179,568.00
Total Price				475,090.00
Notes: Hi-Care Premier On-Site Service include: 7*24 Technical Assistance Center Access. Access to all new software updates and Online Support. 24*7*4 Hours Onsite Hardware Replacement				

The above pricing includes hardware maintenance and software support for three years, 7 days per week, 24 hours per day. The hardware maintenance and software support provides the following:

- Acknowledgement of new and existing problems with four (4) hours.
- Onsite presence of a qualified maintenance engineer or provision of a customer replaceable part within four (4) hours of the above acknowledgement for any hardware failure that results in an inoperative Price Storage Configuration that can be remedied by the repair or replacement of a Priced Storage Configuration component.

Huawei Technologies Co., Ltd. only sells its products to third-party resellers, who in turn, sell those products to U.S. customers. The above pricing, which also includes the required three-year maintenance and support, was obtained from one of those third-party resellers. See page 75 (*“Appendix F: Third-Party Quotation”*) for a copy of the third-party reseller quotation.

Priced Storage Configuration Diagram

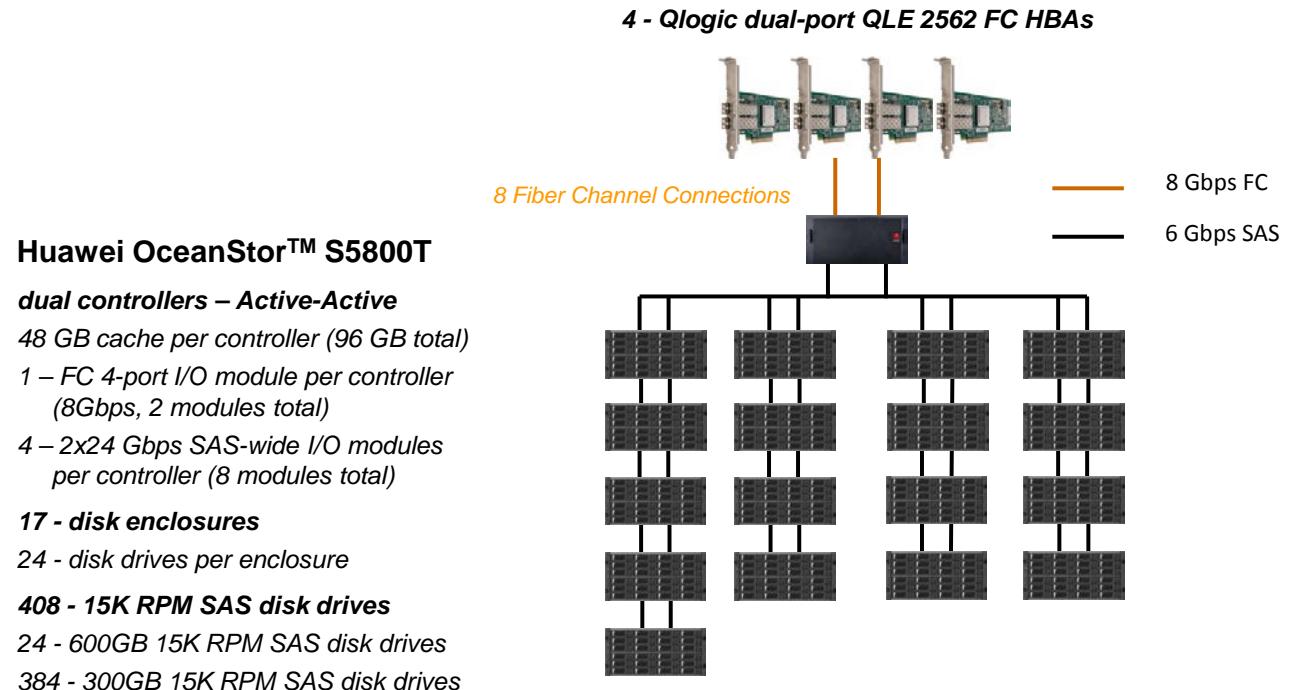

Priced Storage Configuration Components

Priced Storage Configuration:
4 – Qlogic dual-port QLE2562 FC HBAs
Huawei OceanStor™ S5800T
dual controllers – Active-Active
<ul style="list-style-type: none"> 48 GB cache per controller (96 GB total) 1 – FC 4-port I/O module per controller (8 Gbps, 2 modules total) 4 – 8 Gbps front-end connections per controller (8 total, 8 used) 4 – 2x24 Gbps SAS-wide I/O modules per controller (8 total) (2 ports per modules) 8 – 2x24 Gbps SAS backend connections per controller (16 total, 8 used)
17 – Disk Enclosures
<ul style="list-style-type: none"> 24 – 3.5" HD slots per enclosure 24 – disk drives in each enclosures
408 – 15K RPM SAS disk drives
<ul style="list-style-type: none"> 384 – 300 GB disk drives 24 – 600 GB disk drives

In each of the following sections of this document, the appropriate Full Disclosure Report requirement, from the SPC-1 benchmark specification, is stated in italics followed by the information to fulfill the stated requirement.

CONFIGURATION INFORMATION

Benchmark Configuration (BC)/Tested Storage Configuration (TSC) Diagram

Clause 9.4.3.4.1

A one page Benchmark Configuration (BC)/Tested Storage Configuration (TSC) diagram shall be included in the FDR...

The Benchmark Configuration (BC)/Tested Storage Configuration (TSC) is illustrated on page 18 (*Benchmark Configuration/Tested Storage Configuration Diagram*).

Storage Network Configuration

Clause 9.4.3.4.1

...

5. *If the TSC contains network storage, the diagram will include the network configuration. If a single diagram is not sufficient to illustrate both the Benchmark Configuration and network configuration in sufficient detail, the Benchmark Configuration diagram will include a high-level network illustration as shown in Figure 9-8. In that case, a separate, detailed network configuration diagram will also be included as described in Clause 9.4.3.4.2.*

Clause 9.4.3.4.2

If a storage network was configured as a part of the Tested Storage Configuration and the Benchmark Configuration diagram described in Clause 9.4.3.4.1 contains a high-level illustration of the network configuration, the Executive Summary will contain a one page topology diagram of the storage network as illustrated in Figure 9-9.

The Benchmark Configuration (BC)/Tested Storage Configuration (TSC) was configured with local storage and, as such, did not employ a storage network.


Host System(s) and Tested Storage Configuration (TSC) Table of Components

Clause 9.4.3.4.3

The FDR will contain a table that lists the major components of each Host System and the Tested Storage Configuration (TSC). Table 9-10 specifies the content, format, and appearance of the table.

The Host System(s) and TSC table of components may be found on page 18 (*Host Systems and Tested Storage Configuration Components*).

Benchmark Configuration/Tested Storage Configuration Diagram

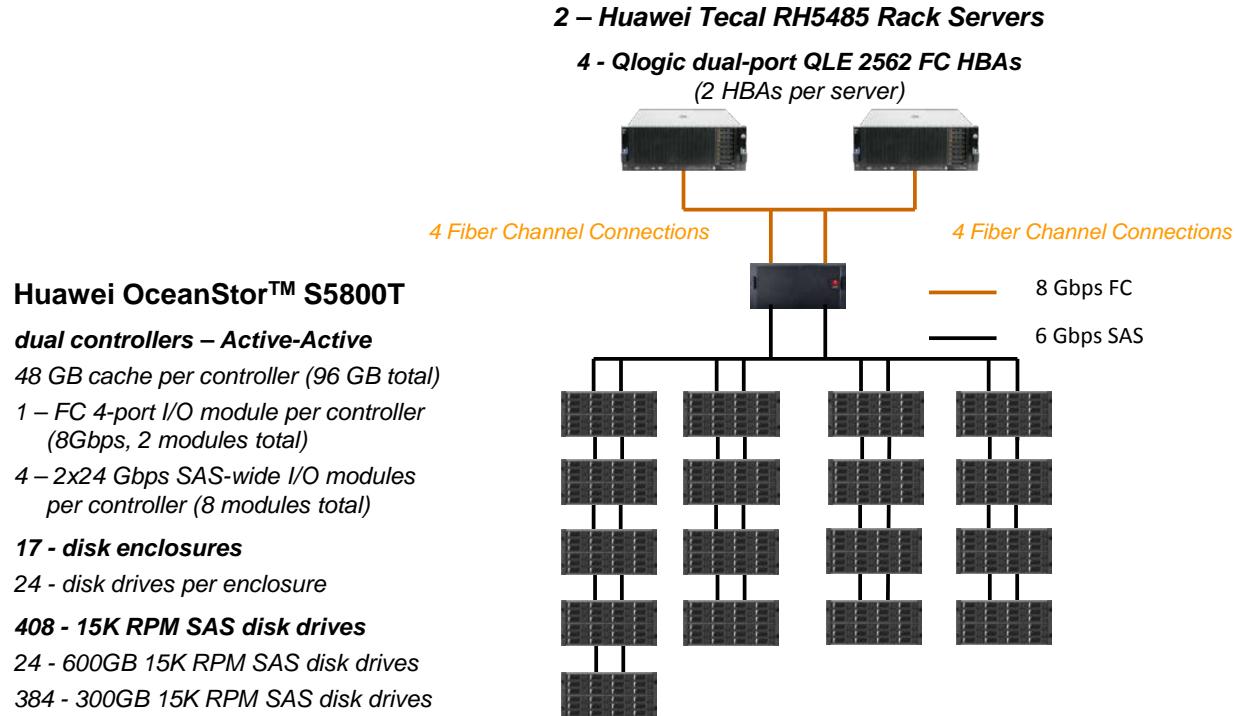

Host Systems and Tested Storage Configuration Components

Host Systems:	Tested Storage Configuration (TSC):
2 – Huawei Tecal RH5485 Rack Servers each server with: 4 – Intel Xeon E7530 1.87 GHz CPUs 128 GB main memory Red Hat Enterprise Linux 5.5 x86_64 LVM version 2.02.56(1) PCIe	4 – QLogic dual-ported QLE2562 FC HBAs
	Huawei OceanStor™ S5800T dual controllers – Active-Active 48 GB cache per controller (96 GB total) 1 – FC 4-port I/O module per controller (8 Gbps, 2 modules total) 4 – 8Gbps front-end connections per controller (8 total, 8 used) 4 – 2x24 Gbps SAS-wide I/O modules per controller (8 modules total, 2 ports per modules) 8 – 2x24 Gbps SAS-wide backend connections per controller (16 total and 8 used)
	17 –Disk Enclosures 24 – 3.5" HD slots per enclosure 24 – disk drives per enclosure
	408 – 15K RPM SAS disk drives 384 – 300 GB disk drives 24 – 600 GB disk drives

Customer Tunable Parameters and Options

Clause 9.4.3.5.1

All Benchmark Configuration (BC) components with customer tunable parameter and options that have been altered from their default values must be listed in the FDR. The FDR entry for each of those components must include both the name of the component and the altered value of the parameter or option. If the parameter name is not self-explanatory to a knowledgeable practitioner, a brief description of the parameter's use must also be included in the FDR entry.

“Appendix B: Customer Tunable Parameters and Options” on page 61 contains the customer tunable parameters and options that have been altered from their default values for this benchmark.

Tested Storage Configuration (TSC) Description

Clause 9.4.3.5.2

The FDR must include sufficient information to recreate the logical representation of the TSC. In addition to customer tunable parameters and options (Clause 4.2.4.5.3), that information must include, at a minimum:

- *A diagram and/or description of the following:*
 - *All physical components that comprise the TSC. Those components are also illustrated in the BC Configuration Diagram in Clause 9.2.4.4.1 and/or the Storage Network Configuration Diagram in Clause 9.2.4.4.2.*
 - *The logical representation of the TSC, configured from the above components that will be presented to the Workload Generator.*
- *Listings of scripts used to create the logical representation of the TSC.*
- *If scripts were not used, a description of the process used with sufficient detail to recreate the logical representation of the TSC.*

“Appendix C: Tested Storage Configuration (TSC) Creation” on page 62 contains the detailed information that describes how to create and configure the logical TSC.

SPC-1 Workload Generator Storage Configuration

Clause 9.4.3.5.3

The FDR must include all SPC-1 Workload Generator storage configuration commands and parameters.

The SPC-1 Workload Generator storage configuration commands and parameters for this measurement appear in “Appendix D: SPC-1 Workload Generator Storage Commands and Parameters” on page 69.

ASU Pre-Fill

Clause 5.3.3

Each of the three SPC-1 ASUs (ASU-1, ASU-2 and ASU-3) is required to be completely filled with specified content prior to the execution of audited SPC-1 Tests. The content is required to consist of random data pattern such as that produced by an SPC recommended tool.

The configuration file used to complete the required ASU pre-fill appears in “*Appendix D: SPC-1 Workload Generator Storage Commands and Parameters*” on page 69.

SPC-1 DATA REPOSITORY

This portion of the Full Disclosure Report presents the detailed information that fully documents the various SPC-1 storage capacities and mappings used in the Tested Storage Configuration. “SPC-1 Data Repository Definitions” on page 57 contains definitions of terms specific to the SPC-1 Data Repository.

Storage Capacities and Relationships

Clause 9.4.3.6.1

Two tables and an illustration documenting the storage capacities and relationships of the SPC-1 Storage Hierarchy (Clause 2.1) shall be included in the FDR.

SPC-1 Storage Capacities


The Physical Storage Capacity consisted of 129,603.054 GB distributed over 384 disk drives, each with a formatted capacity of 300.00 GB and 24 disk drives, each with a formatted capacity of 600.127 GB. There was 197.568 GB (0.15%) of Unused Storage within the Physical Storage Capacity. Global Storage Overhead consisted of 327.760 GB (0.25%) of the Physical Storage Capacity. There was 28,145.994 GB (21.81%) of Unused Storage within the Configured Storage Capacity. The Total ASU Capacity utilized 100% of the Addressable Storage Capacity resulting in 0.00 GB (0.00%) of Unused Storage within the Addressable Storage Capacity. The Data Protection (*Mirroring*) capacity was 64,538.863 GB of which 50,465.866 GB was utilized. The total Unused Storage capacity was 28,343.563 GB.

Note: The configured Storage Devices may include additional storage capacity reserved for system overhead, which is not accessible for application use. That storage capacity may not be included in the value presented for Physical Storage Capacity.

SPC-1 Storage Capacities		
Storage Hierarchy Component	Units	Capacity
Total ASU Capacity	Gigabytes (GB)	50,465.866
Addressable Storage Capacity	Gigabytes (GB)	50,465.866
Configured Storage Capacity	Gigabytes (GB)	129,077.726
Physical Storage Capacity	Gigabytes (GB)	129,603.054
Data Protection (<i>Mirroring</i>)	Gigabytes (GB)	64,538.863
Required Storage	Gigabytes (GB)	0.000
Global Storage Overhead	Gigabytes (GB)	327.760
Total Unused Storage	Gigabytes (GB)	28,343.563

SPC-1 Storage Capacities and Relationships Illustration

The various storage capacities configured in the benchmark result are illustrated below (*not to scale*).

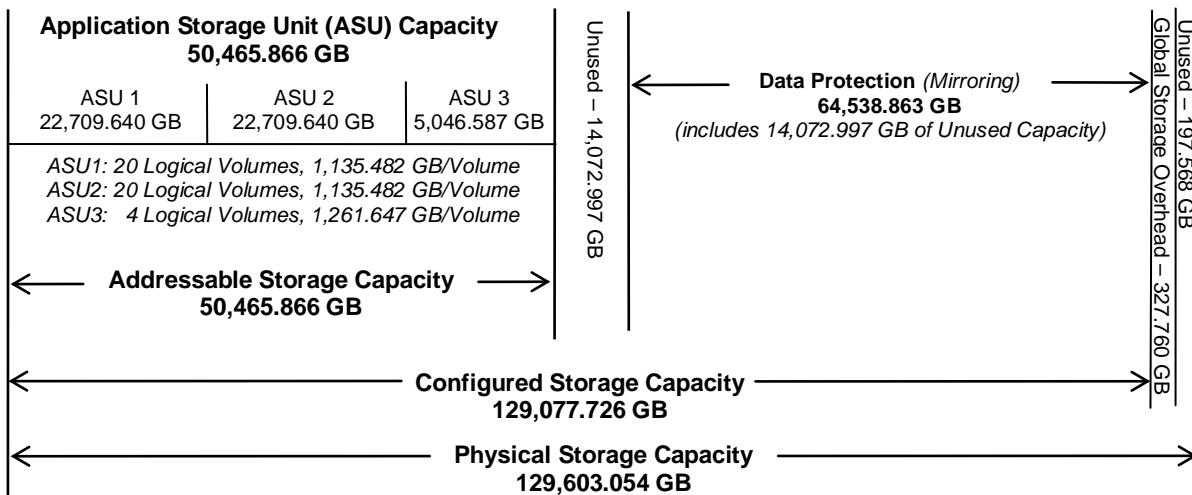

SPC-1 Storage Hierarchy Ratios

	Addressable Storage Capacity	Configured Storage Capacity	Physical Storage Capacity
Total ASU Capacity	100.00%	39.10%	38.94%
Required for Data Protection (Mirroring)		50.00%	49.80%
Addressable Storage Capacity		39.10%	38.94%
Required Storage		0.00%	0.00%
Configured Storage Capacity			99.59%
Global Storage Overhead			0.25%
Unused Storage:			
Addressable	0.00%		
Configured		21.81%	
Physical			0.15%

Storage Capacity Utilization

Clause 9.4.3.6.2

The FDR will include a table illustrating the storage capacity utilization values defined for Application Utilization (Clause 2.8.1), Protected Application Utilization (Clause 2.8.2), and Unused Storage Ratio (Clause 2.8.3).

Clause 2.8.1

Application Utilization is defined as Total ASU Capacity divided by Physical Storage Capacity.

Clause 2.8.2

Protected Application Utilization is defined as (Total ASU Capacity plus total Data Protection Capacity minus unused Data Protection Capacity) divided by Physical Storage Capacity.

Clause 2.8.3

Unused Storage Ratio is defined as Total Unused Capacity divided by Physical Storage Capacity and may not exceed 45%.

SPC-1 Storage Capacity Utilization	
Application Utilization	38.94%
Protected Application Utilization	77.88%
Unused Storage Ratio	21.87%

Logical Volume Capacity and ASU Mapping

Clause 9.4.3.6.3

A table illustrating the capacity of each ASU and the mapping of Logical Volumes to ASUs shall be provided in the FDR. ... Logical Volumes shall be sequenced in the table from top to bottom per its position in the contiguous address space of each ASU. The capacity of each Logical Volume shall be stated. ... In conjunction with this table, the Test Sponsor shall provide a complete description of the type of data protection (see Clause 2.4.5) used on each Logical Volume.

Logical Volume Capacity and Mapping		
ASU-1 (22,709.640 GB)	ASU-2 (22,709.640 GB)	ASU-3 (5,046.587 GB)
20 Logical Volumes 1,135.482 per Logical Volume (1,135.482 GB used per Logical Volume)	20 Logical Volumes 1,135.482 per Logical Volume (1,135.482 GB used per Logical Volume)	4 Logical Volumes 1,261.647 per Logical Volume (1,261.647 GB used per Logical Volume)

The Data Protection Level used for all Logical Volumes was **Protected 1** using **Mirroring** as described on page 11. See “ASU Configuration” in the [IOPS Test Results File](#) for more detailed configuration information.

SPC-1 BENCHMARK EXECUTION RESULTS

This portion of the Full Disclosure Report documents the results of the various SPC-1 Tests, Test Phases, and Test Runs. “**Protected 1:** The single point of failure of any **storage device** in the configuration will not result in permanent loss of access to or integrity of the SPC-1 Data Repository.

Protected 2: The single point of failure of any **component** in the configuration will not result in permanent loss of access to or integrity of the SPC-1 Data Repository.

SPC-1 Test Execution Definitions” on page 58 contains definitions of terms specific to the SPC-1 Tests, Test Phases, and Test Runs.

Clause 5.4.3

The Tests must be executed in the following sequence: Primary Metrics, Repeatability, and Data Persistence. That required sequence must be uninterrupted from the start of Primary Metrics to the completion of Persistence Test Run 1. Uninterrupted means the Benchmark Configuration shall not be power cycled, restarted, disturbed, altered, or adjusted during the above measurement sequence. If the required sequence is interrupted other than for the Host System/TSC power cycle between the two Persistence Test Runs, the measurement is invalid.

SPC-1 Tests, Test Phases, and Test Runs

The SPC-1 benchmark consists of the following Tests, Test Phases, and Test Runs:

- **Primary Metrics Test**
 - Sustainability Test Phase and Test Run
 - IOPS Test Phase and Test Run
 - Response Time Ramp Test Phase
 - 95% of IOPS Test Run
 - 90% of IOPS Test Run
 - 80% of IOPS Test Run
 - 50% of IOPS Test Run
 - 10% of IOPS Test Run (LRT)
- **Repeatability Test**
 - Repeatability Test Phase 1
 - 10% of IOPS Test Run (LRT)
 - IOPS Test Run
 - Repeatability Test Phase 2
 - 10% of IOPS Test Run (LRT)
 - IOPS Test Run
- **Data Persistence Test**
 - Data Persistence Test Run 1
 - Data Persistence Test Run 2

Each Test is an atomic unit that must be executed from start to finish before any other Test, Test Phase, or Test Run may be executed.

The results from each Test, Test Phase, and Test Run are listed below along with a more detailed explanation of each component.

Primary Metrics Test – Sustainability Test Phase

Clause 5.4.4.1.1

The Sustainability Test Phase has exactly one Test Run and shall demonstrate the maximum sustainable I/O Request Throughput within at least a continuous eight (8) hour Measurement Interval. This Test Phase also serves to insure that the TSC has reached Steady State prior to reporting the final maximum I/O Request Throughput result (SPC-1 IOPSTM).

Clause 5.4.4.1.2

The computed I/O Request Throughput of the Sustainability Test must be within 5% of the reported SPC-1 IOPSTM result.

Clause 5.4.4.1.4

The Average Response Time, as defined in Clause 5.1.1, will be computed and reported for the Sustainability Test Run and cannot exceed 30 milliseconds. If the Average Response time exceeds that 30-milliseconds constraint, the measurement is invalid.

Clause 9.4.3.7.1

For the Sustainability Test Phase the FDR shall contain:

1. *A Data Rate Distribution graph and data table.*
2. *I/O Request Throughput Distribution graph and data table.*
3. *A Response Time Frequency Distribution graph and table.*
4. *An Average Response Time Distribution graph and table.*
5. *The human readable Test Run Results File produced by the Workload Generator (may be included in an appendix).*
6. *A listing or screen image of all input parameters supplied to the Workload Generator (may be included in an appendix).*
7. *The Measured Intensity Multiplier for each I/O stream.*
8. *The variability of the Measured Intensity Multiplier, as defined in Clause 5.3.13.3.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 72.

Sustainability Test Results File

A link to the test results file generated from the Sustainability Test Run is listed below.


[Sustainability Test Results File](#)

Sustainability – Data Rate Distribution Data (*MB/second*)

The Sustainability Data Rate table of data is not embedded in this document due to its size. The table is available via the following URL:

[Sustainability Data Rate Table](#)

Sustainability – Data Rate Distribution Graph

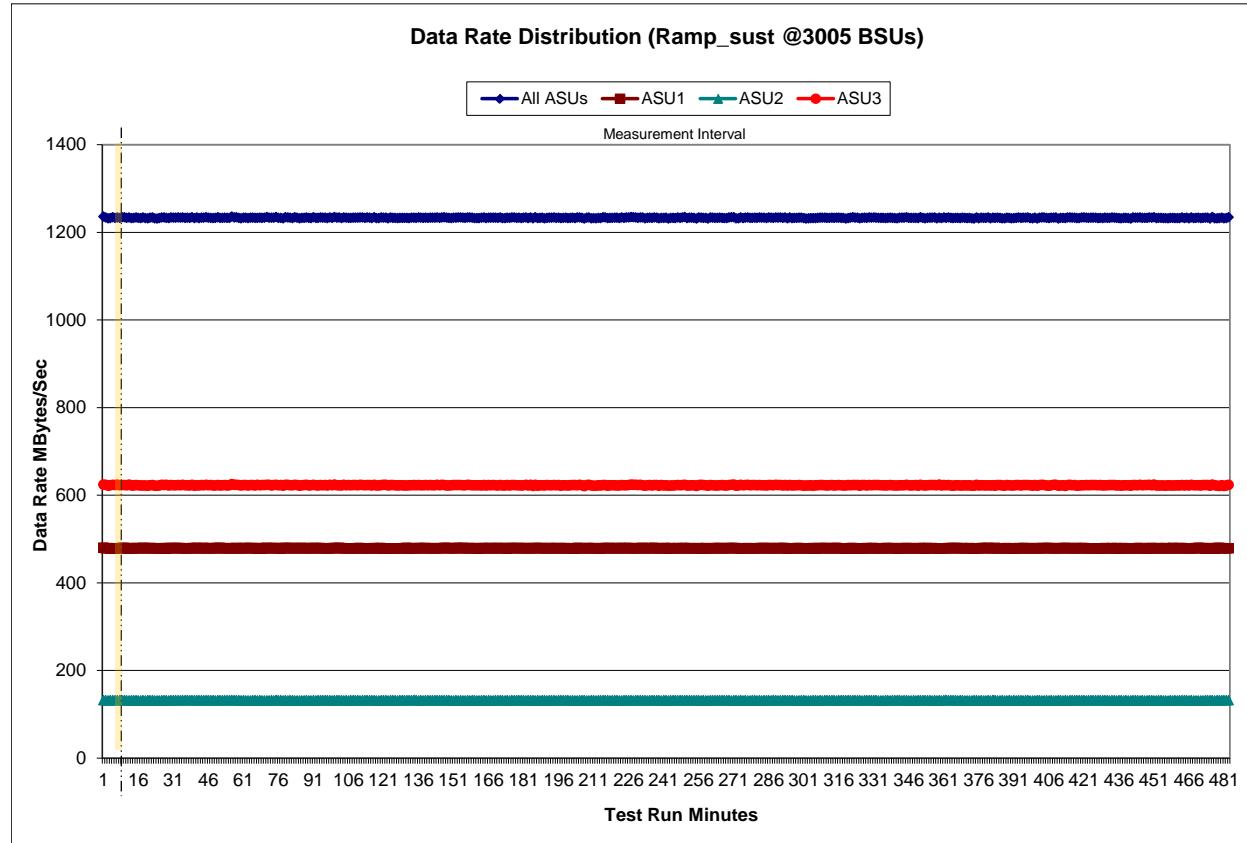


Sustainability – I/O Request Throughput Distribution Data

The Sustainability I/O Request Throughput table of data is not embedded in this document due to its size. The table is available via the following URL:

[Sustainability I/O Request Throughput Table](#)

Sustainability – I/O Request Throughput Distribution Graph

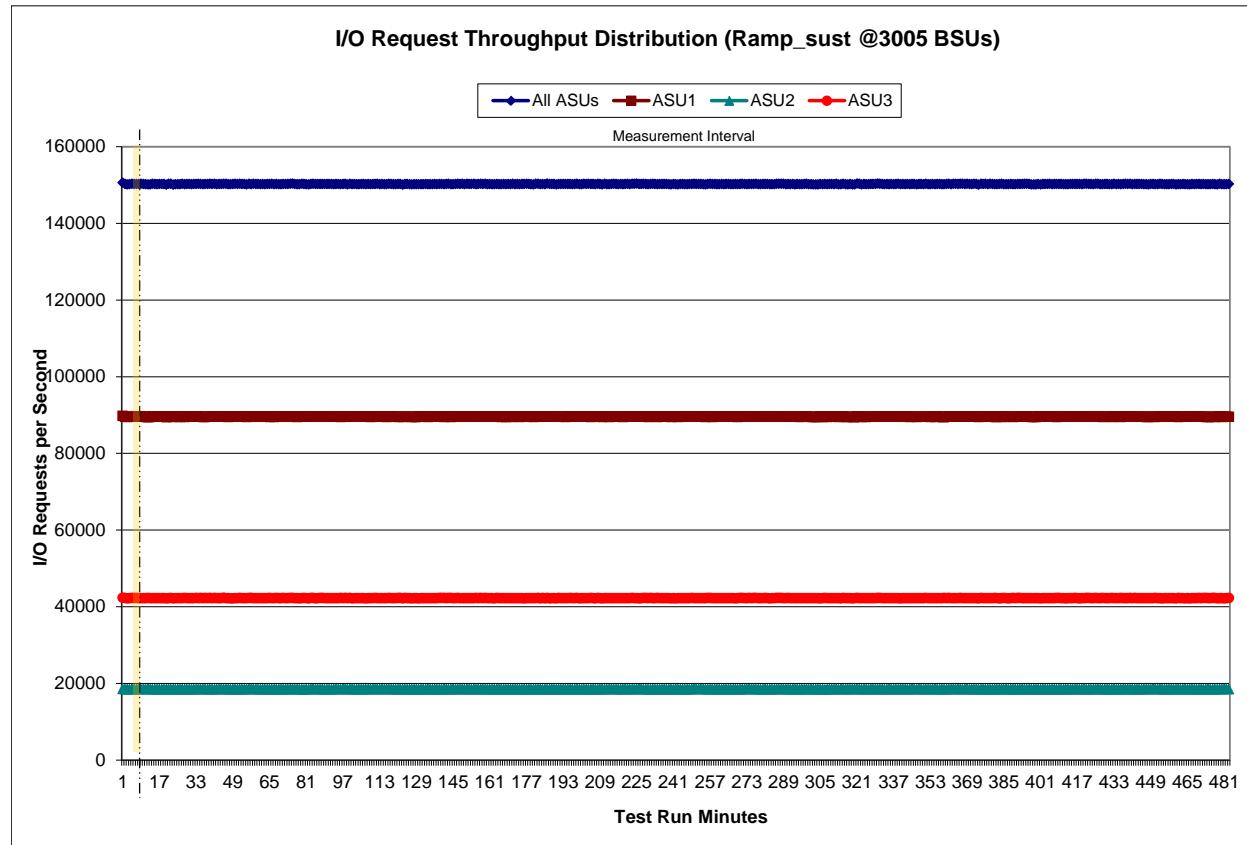


Sustainability – Average Response Time (ms) Distribution Data

The Sustainability Average Response Time table of data is not embedded in this document due to its size. The table is available via the following URL:

[Sustainability Average Response Time Table](#)


Sustainability – Average Response Time (ms) Distribution Graph

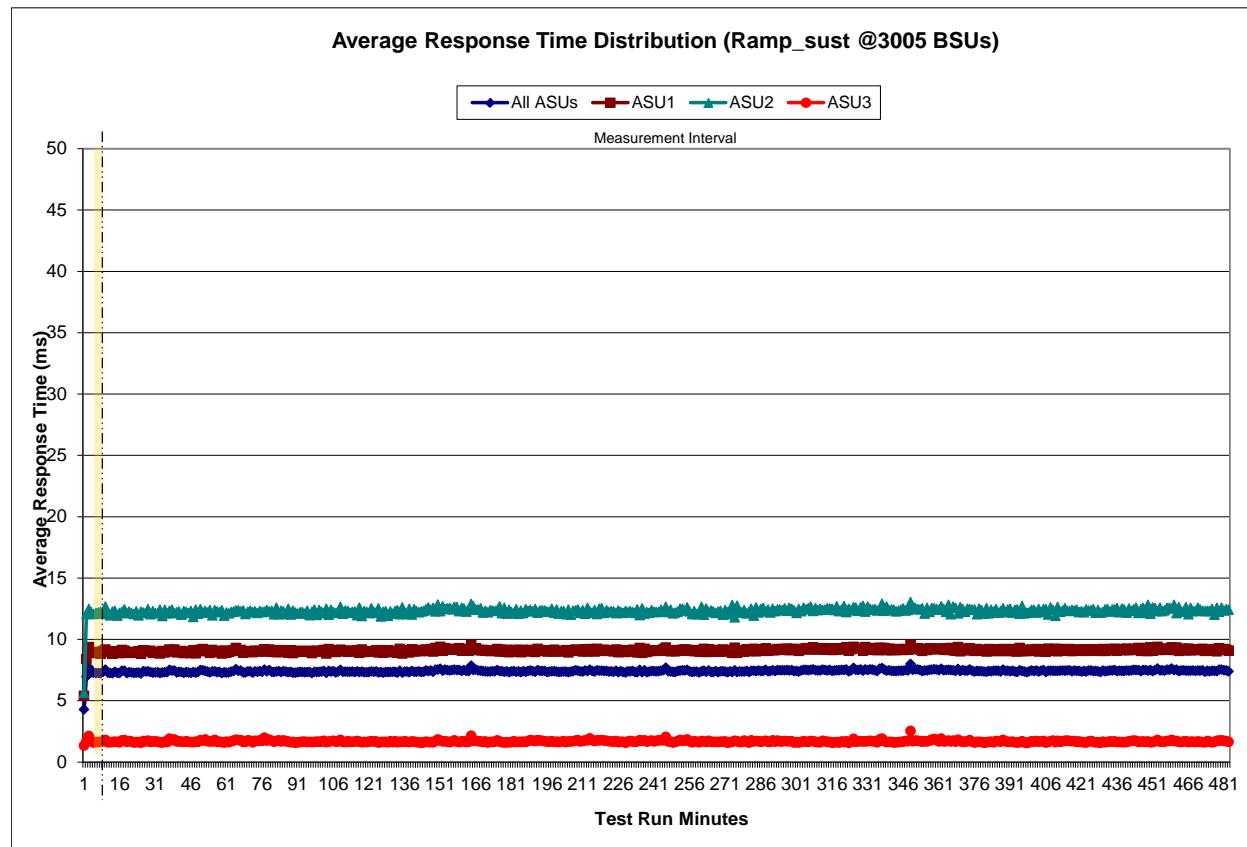

Sustainability – Response Time Frequency Distribution Data

Response Time (ms)	0-0.25	>0.25-0.5	>0.5-0.75	>0.75-1.0	>1.0-1.25	>1.25-1.5	>1.5-1.75	>1.75-2.0
Read	125,021,188	35,693,116	6,760,345	5,876,921	8,013,464	8,248,977	7,288,186	7,528,579
Write	13,762	82,921,592	360,695,905	474,286,631	498,336,175	352,005,221	217,086,643	158,148,399
All ASUs	125,034,950	118,614,708	367,456,250	480,163,552	506,349,639	360,254,198	224,374,829	165,676,978
ASU1	102,632,696	67,903,351	167,363,456	212,900,726	223,347,789	158,548,893	98,803,246	73,448,796
ASU2	22,396,582	15,188,462	38,718,765	49,723,788	52,377,769	37,213,994	23,159,024	17,130,768
ASU3	5,672	35,522,895	161,374,029	217,539,038	230,624,081	164,491,311	102,412,559	75,097,414
Response Time (ms)	>2.0-2.5	>2.5-3.0	>3.0-3.5	>3.5-4.0	>4.0-4.5	>4.5-5.0	>5.0-6.0	>6.0-7.0
Read	18,066,015	16,340,842	22,764,154	23,849,552	35,093,732	36,771,868	100,416,650	118,814,138
Write	226,359,910	86,509,588	58,838,794	27,836,555	21,743,469	12,042,273	15,510,107	7,326,494
All ASUs	244,425,925	102,850,430	81,602,948	51,686,107	56,837,201	48,814,141	115,926,757	126,140,632
ASU1	111,749,032	51,175,597	45,696,948	33,946,460	42,026,920	39,441,435	99,263,293	110,503,003
ASU2	25,448,600	10,525,570	7,969,669	4,530,287	4,504,733	3,648,360	9,256,577	12,102,299
ASU3	107,228,293	41,149,263	27,936,331	13,209,360	10,305,548	5,724,346	7,406,887	3,535,330
Response Time (ms)	>7.0-8.0	>8.0-9.0	>9.0-10.0	>10.0-15.0	>15.0-20.0	>20.0-25.0	>25.0-30.0	>30.0
Read	121,887,879	109,239,754	91,092,785	258,321,001	129,595,157	87,211,455	64,939,300	267,754,022
Write	3,821,552	2,248,266	1,590,462	4,425,564	1,861,289	1,302,557	982,747	4,670,231
All ASUs	125,709,431	111,488,020	92,683,247	262,746,565	131,456,446	88,514,012	65,922,047	272,424,253
ASU1	109,367,914	94,978,942	77,790,734	220,311,583	110,624,658	73,671,077	54,144,953	199,334,418
ASU2	14,474,052	15,388,620	14,086,493	40,078,383	19,695,315	13,986,704	11,092,613	69,538,851
ASU3	1,867,465	1,120,458	806,020	2,356,599	1,136,473	856,231	684,481	3,550,984

Sustainability – Response Time Frequency Distribution Graph

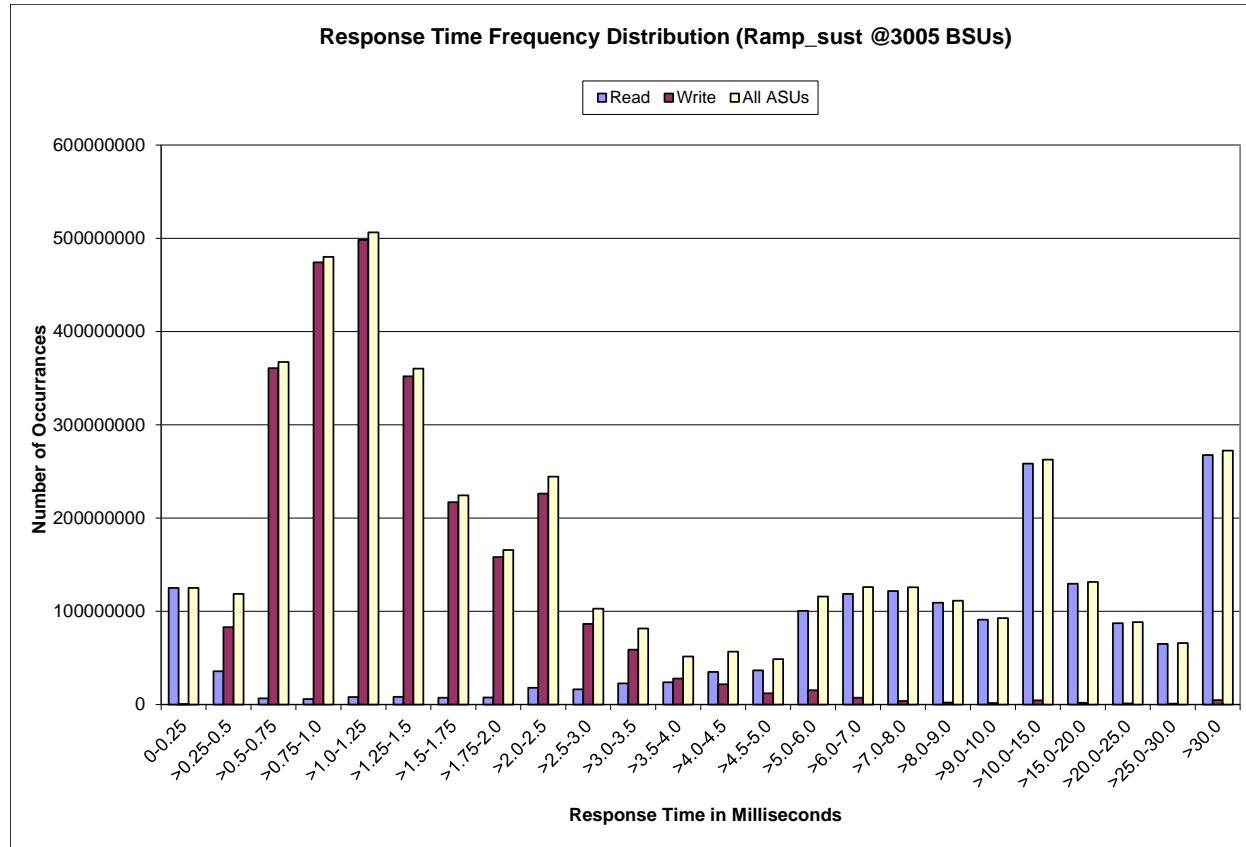

Sustainability – Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.15.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.15.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
COV	0.002	0.001	0.001	0.001	0.003	0.001	0.002	0.001

Primary Metrics Test – IOPS Test Phase

Clause 5.4.4.2

The IOPS Test Phase consists of one Test Run at the 100% load point with a Measurement Interval of ten (10) minutes. The IOPS Test Phase immediately follows the Sustainability Test Phase without any interruption or manual intervention.

The IOPS Test Run generates the SPC-1 IOPSTM primary metric, which is computed as the I/O Request Throughput for the Measurement Interval of the IOPS Test Run.

The Average Response Time is computed for the IOPS Test Run and cannot exceed 30 milliseconds. If the Average Response Time exceeds the 30 millisecond constraint, the measurement is invalid.

Clause 9.4.3.7.2

For the IOPS Test Phase the FDR shall contain:

1. *I/O Request Throughput Distribution (data and graph).*
2. *A Response Time Frequency Distribution.*
3. *An Average Response Time Distribution.*
4. *The human readable Test Run Results File produced by the Workload Generator.*
5. *A listing or screen image of all input parameters supplied to the Workload Generator.*
6. *The total number of I/O Requests completed in the Measurement Interval as well as the number of I/O Requests with a Response Time less than or equal to 30 milliseconds and the number of I/O Requests with a Response Time greater than 30 milliseconds.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 72.

IOPS Test Results File


A link to the test results file generated from the IOPS Test Run is listed below.

[IOPS Test Results File](#)

IOPS Test Run – I/O Request Throughput Distribution Data

3,005 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	19:52:08	19:55:09	0-2	0:03:01
Measurement Interval	19:55:09	20:05:09	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	150,557.70	89,751.77	18,516.57	42,289.37
1	150,252.78	89,590.60	18,462.13	42,200.05
2	150,176.40	89,455.87	18,511.78	42,208.75
3	150,291.82	89,598.18	18,492.65	42,200.98
4	150,370.88	89,602.07	18,486.95	42,281.87
5	150,250.82	89,502.12	18,504.38	42,244.32
6	150,239.52	89,521.20	18,494.27	42,224.05
7	150,366.32	89,582.90	18,485.53	42,297.88
8	150,237.50	89,555.15	18,465.58	42,216.77
9	150,241.58	89,591.23	18,452.47	42,197.88
10	150,327.35	89,579.50	18,503.77	42,244.08
11	150,281.38	89,584.35	18,462.75	42,234.28
12	150,255.33	89,519.53	18,488.43	42,247.37
Average	150,286.25	89,563.62	18,483.68	42,238.95


IOPS Test Run – I/O Request Throughput Distribution Graph

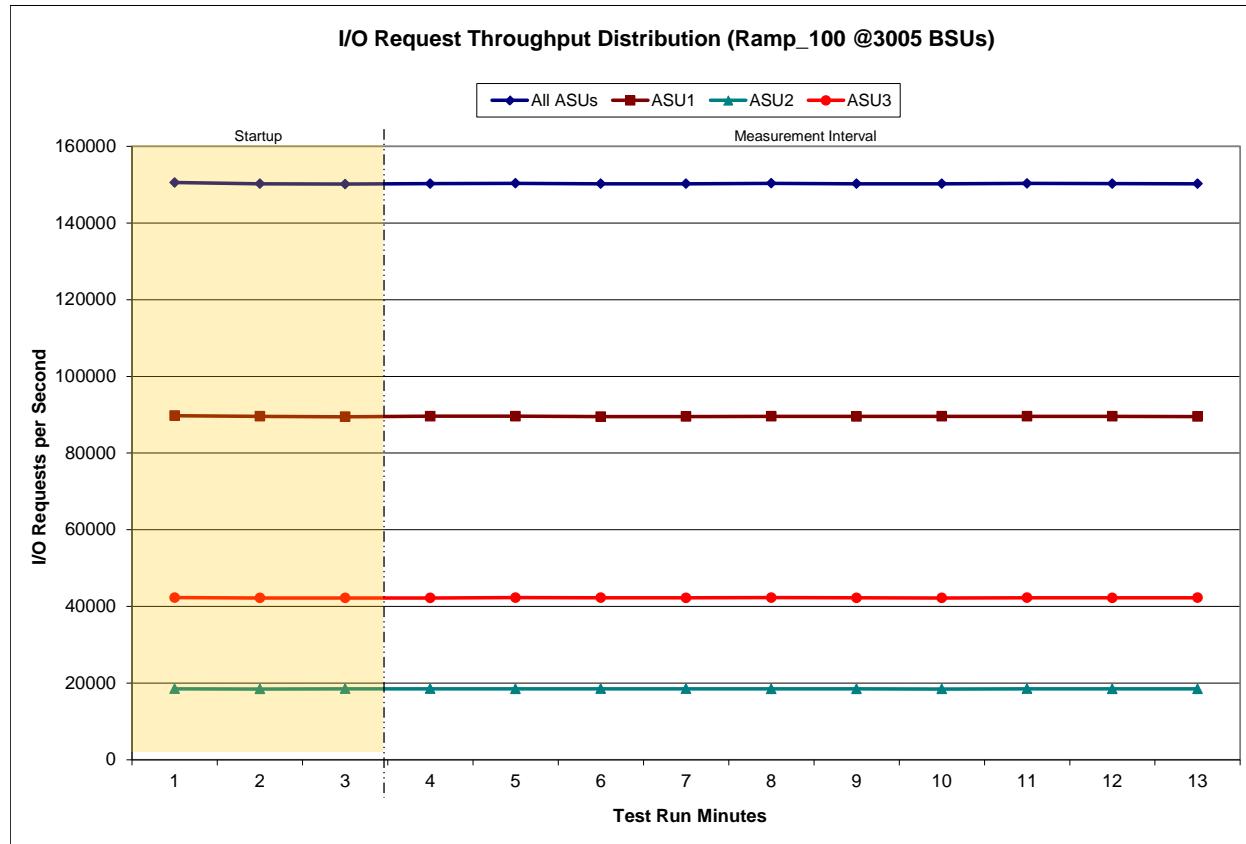

IOPS Test Run – Average Response Time (ms) Distribution Data

3,005 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	19:52:08	19:55:09	0-2	0:03:01
Measurement Interval	19:55:09	20:05:09	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	7.47	9.07	12.36	1.95
1	7.50	9.18	12.33	1.80
2	7.76	9.37	12.77	2.14
3	7.49	9.19	12.23	1.78
4	7.44	9.07	12.51	1.77
5	7.37	9.06	12.20	1.70
6	7.34	8.99	12.20	1.72
7	7.32	8.96	12.30	1.69
8	7.41	9.07	12.40	1.73
9	7.41	9.06	12.31	1.77
10	7.34	8.99	12.27	1.69
11	7.40	9.05	12.23	1.77
12	7.28	8.89	12.25	1.69
Average	7.38	9.03	12.29	1.73


IOPS Test Run – Average Response Time (ms) Distribution Graph

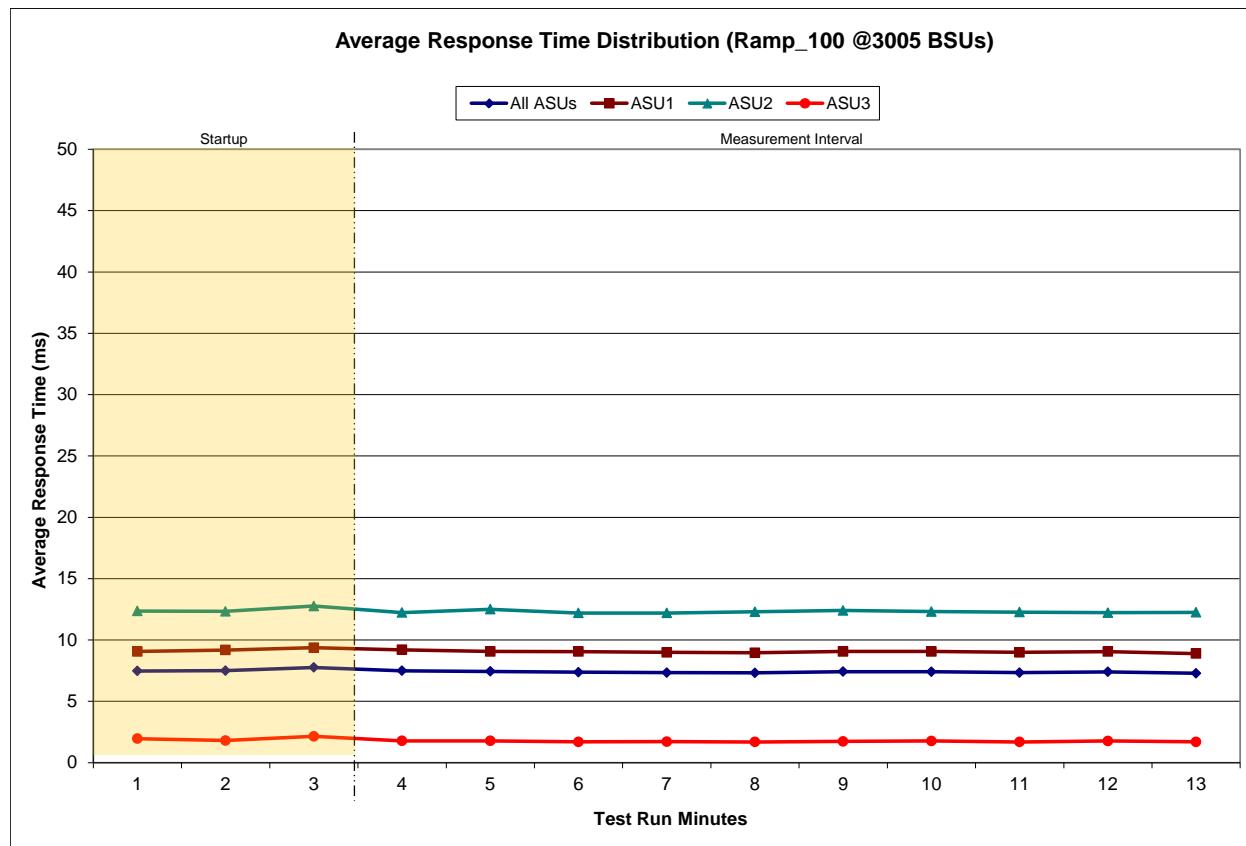

IOPS Test Run – Response Time Frequency Distribution Data

Response Time (ms)	0-0.25	>0.25-0.5	>0.5-0.75	>0.75-1.0	>1.0-1.25	>1.25-1.5	>1.5-1.75	>1.75-2.0
Read	2,700,620	831,534	162,447	124,563	167,619	171,577	152,165	154,175
Write	249	1,658,225	7,391,229	9,684,722	10,299,451	7,392,613	4,592,048	3,291,431
All ASUs	2,700,869	2,489,759	7,553,676	9,809,285	10,467,070	7,564,190	4,744,213	3,445,606
ASU1	2,242,905	1,464,856	3,454,415	4,351,947	4,618,296	3,330,887	2,088,207	1,526,238
ASU2	457,863	317,272	796,685	1,016,989	1,082,010	780,839	491,129	355,018
ASU3	101	707,631	3,302,576	4,440,349	4,766,764	3,452,464	2,164,877	1,564,350
Response Time (ms)	>2.0-2.5	>2.5-3.0	>3.0-3.5	>3.5-4.0	>4.0-4.5	>4.5-5.0	>5.0-6.0	>6.0-7.0
Read	377,574	340,994	478,407	497,433	737,653	769,502	2,104,257	2,492,304
Write	4,805,635	1,856,516	1,269,383	608,887	477,125	270,489	347,755	163,724
All ASUs	5,183,209	2,197,510	1,747,790	1,106,320	1,214,778	1,039,991	2,452,012	2,656,028
ASU1	2,369,690	1,089,904	973,883	718,755	892,479	832,749	2,088,463	2,319,911
ASU2	538,169	224,769	169,876	97,447	96,464	78,691	197,230	257,189
ASU3	2,275,350	882,837	604,031	290,118	225,835	128,551	166,319	78,928
Response Time (ms)	>7.0-8.0	>8.0-9.0	>9.0-10.0	>10.0-15.0	>15.0-20.0	>20.0-25.0	>25.0-30.0	>30.0
Read	2,557,525	2,282,267	1,885,344	5,244,910	2,658,537	1,799,602	1,340,934	5,520,928
Write	86,030	52,014	38,646	115,343	50,459	32,670	21,466	111,740
All ASUs	2,643,555	2,334,281	1,923,990	5,360,253	2,708,996	1,832,272	1,362,400	5,632,668
ASU1	2,293,725	1,981,410	1,605,778	4,472,185	2,272,441	1,520,857	1,116,525	4,110,905
ASU2	307,761	326,952	298,811	828,339	407,246	290,811	231,048	1,441,404
ASU3	42,069	25,919	19,401	59,729	29,309	20,604	14,827	80,359

IOPS Test Run – Response Time Frequency Distribution Graph

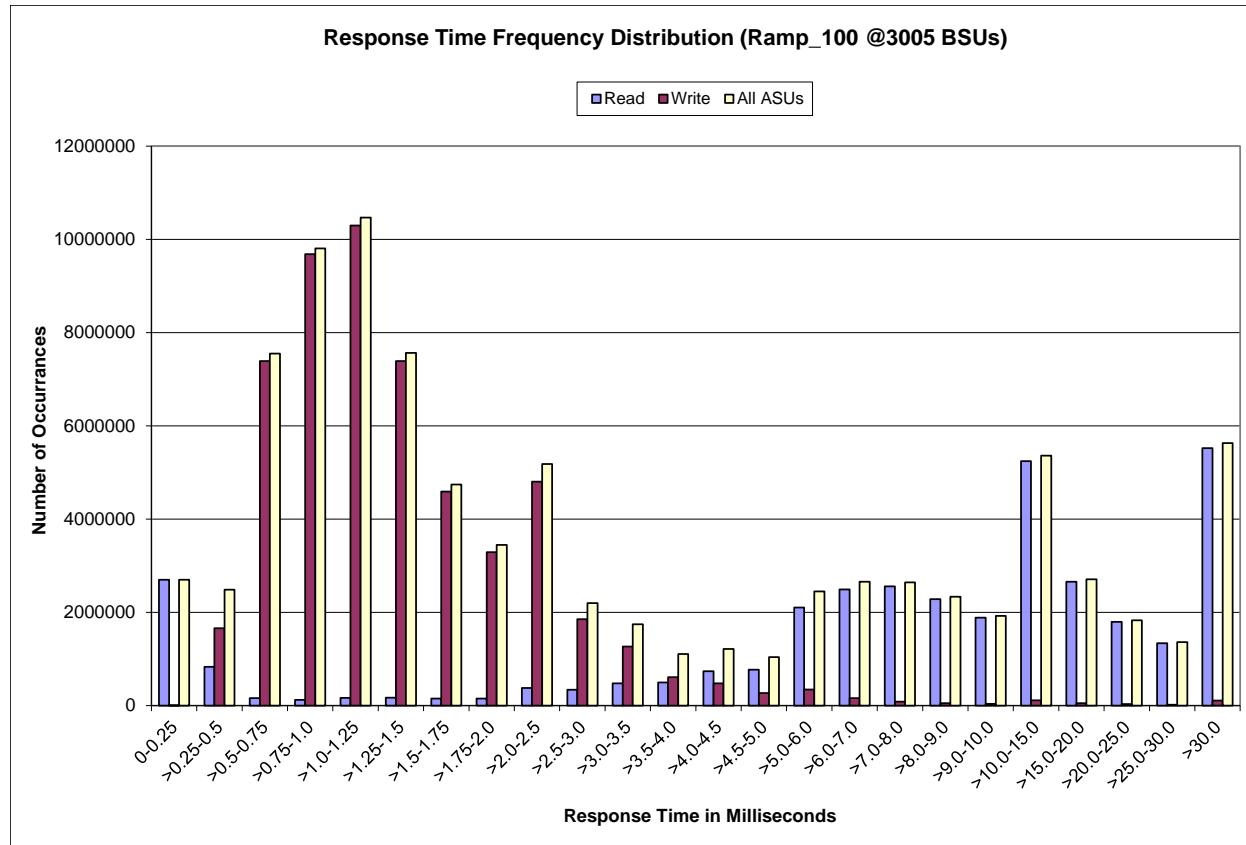

IOPS Test Run – I/O Request Information

I/O Requests Completed in the Measurement Interval	I/O Requests Completed with Response Time = or < 30 ms	I/O Requests Completed with Response Time > 30 ms
90,170,721	84,538,053	5,632,668

IOPS Test Run – Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.15.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.15.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2099	0.0180	0.0700	0.0350	0.2811
COV	0.001	0.001	0.001	0.001	0.002	0.001	0.001	0.001

Primary Metrics Test – Response Time Ramp Test Phase

Clause 5.4.4.3

The Response Time Ramp Test Phase consists of five Test Runs, one each at 95%, 90%, 80%, 50%, and 10% of the load point (100%) used to generate the SPC-1 IOPS™ primary metric. Each of the five Test Runs has a Measurement Interval of ten (10) minutes. The Response Time Ramp Test Phase immediately follows the IOPS Test Phase without any interruption or manual intervention.

The five Response Time Ramp Test Runs, in conjunction with the IOPS Test Run (100%), demonstrate the relationship between Average Response Time and I/O Request Throughput for the Tested Storage Configuration (TSC) as illustrated in the response time/throughput curve on page 13.

In addition, the Average Response Time measured during the 10% Test Run is the value for the SPC-1 LRT™ metric. That value represents the Average Response Time of a lightly loaded TSC.

Clause 9.4.3.7.3

The following content shall appear in the FDR for the Response Time Ramp Phase:

1. *A Response Time Ramp Distribution.*
2. *The human readable Test Run Results File produced by the Workload Generator for each Test Run within the Response Time Ramp Test Phase.*
3. *For the 10% Load Level Test Run (SPC-1 LRT™ metric) an Average Response Time Distribution.*
4. *A listing or screen image of all input parameters supplied to the Workload Generator.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 72.

Response Time Ramp Test Results File

A link to each test result file generated from each Response Time Ramp Test Run listed below.

[95% Load Level](#)

[90% Load Level](#)

[80% Load Level](#)

[50% Load Level](#)


[10% Load Level](#)

Response Time Ramp Distribution (IOPS) Data

The five Test Runs that comprise the Response Time Ramp Phase are executed at 95%, 90%, 80%, 50%, and 10% of the Business Scaling Unit (BSU) load level used to produce the SPC-1 IOPS™ primary metric. The 100% BSU load level is included in the following Response Time Ramp data tables and graphs for completeness.

100% Load Level - 3005 BSUs				Start	Stop	Interval	Duration	95% Load Level - 2854 BSUs				Start	Stop	Interval	Duration
Start-Up/Ramp-Up Measurement Interval				19:52:08	19:55:09	0-2	0:03:01	Start-Up/Ramp-Up Measurement Interval				20:05:46	20:08:47	0-2	0:03:01
(60 second intervals)				All ASUs	ASU-1	ASU-2	ASU-3	(60 second intervals)				All ASUs	ASU-1	ASU-2	ASU-3
0	150,557.70	89,751.77	18,516.57	42,289.37				0	142,796.22	85,091.25	17,575.97	40,129.00			
1	150,252.78	89,590.60	18,462.13	42,200.05				1	142,655.83	85,068.40	17,536.47	40,050.97			
2	150,176.40	89,455.87	18,511.78	42,208.75				2	142,670.75	85,059.85	17,561.43	40,049.47			
3	150,291.82	89,598.18	18,492.65	42,200.98				3	142,770.40	85,108.02	17,552.27	40,110.12			
4	150,370.88	89,602.07	18,486.95	42,281.87				4	142,619.85	84,989.40	17,532.75	40,097.70			
5	150,250.82	89,502.12	18,504.38	42,244.32				5	142,655.65	85,022.82	17,549.97	40,082.87			
6	150,239.52	89,521.20	18,494.27	42,224.05				6	142,642.00	84,999.82	17,560.68	40,081.50			
7	150,366.32	89,582.90	18,485.53	42,297.88				7	142,599.05	84,986.67	17,534.43	40,077.95			
8	150,237.50	89,555.15	18,465.58	42,216.77				8	142,650.43	85,017.77	17,545.62	40,087.05			
9	150,241.58	89,591.23	18,452.47	42,197.88				9	142,752.03	85,071.85	17,599.23	40,080.95			
10	150,327.35	89,579.50	18,503.77	42,244.08				10	142,558.27	84,941.15	17,559.85	40,057.27			
11	150,281.38	89,584.35	18,462.75	42,234.28				11	142,859.42	85,128.92	17,574.82	40,155.68			
12	150,255.33	89,519.53	18,488.43	42,247.37				12	142,666.72	85,047.28	17,529.02	40,090.42			
Average	150,286.25	89,563.62	18,483.68	42,238.95				Average	142,677.38	85,031.37	17,553.86	40,092.15			
90% Load Level - 2704 BSUs				Start	Stop	Interval	Duration	80% Load Level - 2404 BSUs				Start	Stop	Interval	Duration
Start-Up/Ramp-Up Measurement Interval				20:19:24	20:22:25	0-2	0:03:01	Start-Up/Ramp-Up Measurement Interval				20:33:03	20:36:04	0-2	0:03:01
(60 second intervals)				All ASUs	ASU-1	ASU-2	ASU-3	(60 second intervals)				All ASUs	ASU-1	ASU-2	ASU-3
0	135,296.48	80,667.45	16,660.40	37,968.63				0	120,294.78	71,707.55	14,814.43	33,772.80			
1	135,259.25	80,612.67	16,634.63	38,011.95				1	120,236.05	71,664.50	14,790.62	33,780.93			
2	135,233.15	80,619.25	16,627.88	37,986.02				2	120,171.85	71,649.17	14,798.15	33,724.53			
3	135,256.82	80,611.97	16,620.82	38,024.03				3	120,216.05	71,644.60	14,765.82	33,805.63			
4	135,212.98	80,571.67	16,614.90	38,026.42				4	120,187.02	71,640.77	14,755.25	33,791.00			
5	135,206.23	80,584.75	16,649.45	37,972.03				5	120,193.82	71,622.07	14,790.67	33,781.08			
6	135,216.78	80,597.58	16,644.68	37,974.52				6	120,249.07	71,663.47	14,784.73	33,800.87			
7	135,133.18	80,571.80	16,587.20	37,974.18				7	120,201.87	71,632.08	14,782.12	33,787.67			
8	135,139.03	80,542.95	16,598.93	37,997.15				8	120,241.45	71,613.48	14,801.42	33,826.55			
9	135,155.43	80,546.17	16,627.30	37,981.97				9	120,130.05	71,611.52	14,772.15	33,746.38			
10	135,195.88	80,570.88	16,622.13	38,002.87				10	120,158.28	71,632.25	14,785.82	33,740.22			
11	135,264.55	80,593.27	16,635.13	38,036.15				11	120,251.17	71,705.33	14,779.13	33,766.70			
12	135,177.97	80,574.80	16,630.73	37,972.43				12	120,131.78	71,605.92	14,762.95	33,762.92			
Average	135,195.89	80,576.58	16,623.13	37,996.18				Average	120,196.06	71,637.15	14,778.01	33,780.90			
50% Load Level - 1502 BSUs				Start	Stop	Interval	Duration	10% Load Level - 300 BSUs				Start	Stop	Interval	Duration
Start-Up/Ramp-Up Measurement Interval				20:46:39	20:49:40	0-2	0:03:01	Start-Up/Ramp-Up Measurement Interval				21:00:12	21:03:13	0-2	0:03:01
(60 second intervals)				All ASUs	ASU-1	ASU-2	ASU-3	(60 second intervals)				All ASUs	ASU-1	ASU-2	ASU-3
0	75,201.82	44,830.35	9,241.02	21,130.45				0	15,016.37	8,932.90	1,854.52	4,228.95			
1	75,090.62	44,760.62	9,239.00	21,091.00				1	15,017.77	8,953.85	1,837.97	4,225.95			
2	75,098.02	44,741.00	9,229.95	21,127.07				2	14,985.15	8,942.32	1,832.45	4,210.38			
3	75,074.67	44,728.45	9,244.75	21,101.47				3	14,985.08	8,929.60	1,843.95	4,211.53			
4	75,128.32	44,730.52	9,264.70	21,133.10				4	14,977.18	8,927.73	1,840.92	4,208.53			
5	75,112.67	44,747.65	9,234.80	21,130.22				5	14,990.57	8,948.03	1,840.47	4,202.07			
6	75,083.92	44,734.80	9,233.33	21,115.78				6	14,994.58	8,931.20	1,839.75	4,223.63			
7	75,069.95	44,738.28	9,239.85	21,091.82				7	14,984.60	8,938.58	1,835.07	4,210.95			
8	75,080.93	44,754.45	9,230.20	21,096.28				8	14,994.67	8,938.32	1,842.85	4,213.50			
9	75,089.22	44,725.75	9,237.02	21,126.45				9	15,011.23	8,942.78	1,847.30	4,221.15			
10	75,079.10	44,796.30	9,209.57	21,073.23				10	15,020.75	8,949.38	1,848.18	4,223.18			
11	75,069.90	44,719.77	9,236.83	21,113.30				11	15,006.72	8,947.50	1,851.62	4,207.60			
12	75,071.35	44,712.52	9,238.47	21,120.37				12	14,976.02	8,923.37	1,845.37	4,207.28			
Average	75,086.00	44,738.85	9,236.95	21,110.20				Average	14,994.14	8,937.65	1,843.55	4,212.94			


Response Time Ramp Distribution (IOPS) Graph

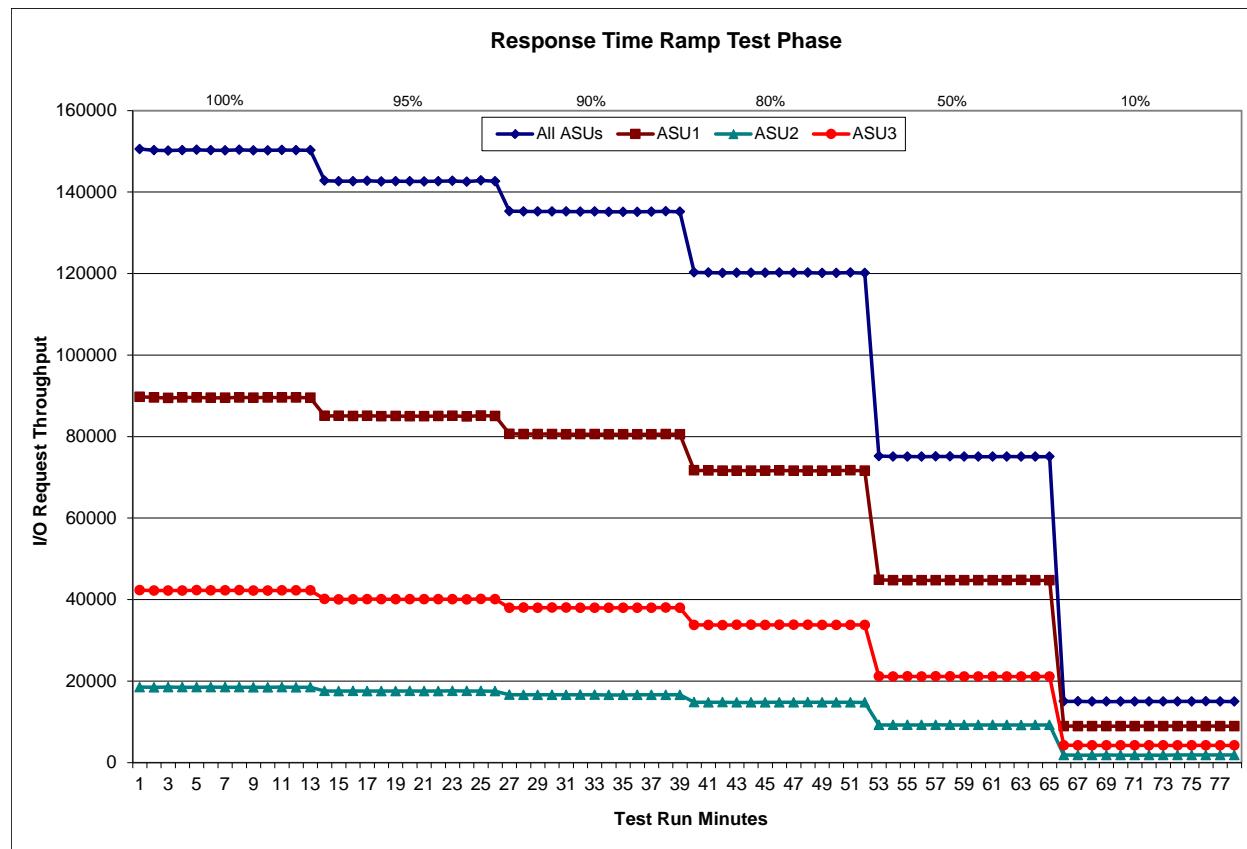

SPC-1 LRT™ Average Response Time (ms) Distribution Data

300 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	21:00:12	21:03:13	0-2	0:03:01
Measurement Interval	21:03:13	21:13:13	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	2.70	3.65	3.29	0.43
1	2.87	3.79	3.43	0.69
2	2.69	3.60	3.22	0.52
3	2.75	3.66	3.27	0.59
4	2.77	3.69	3.28	0.58
5	2.74	3.65	3.22	0.60
6	2.75	3.67	3.24	0.60
7	2.75	3.65	3.27	0.61
8	2.94	3.84	3.46	0.80
9	2.74	3.63	3.32	0.59
10	2.72	3.61	3.27	0.59
11	2.82	3.71	3.37	0.68
12	2.73	3.62	3.29	0.58
Average	2.77	3.67	3.30	0.62

SPC-1 LRT™ Average Response Time (ms) Distribution Graph

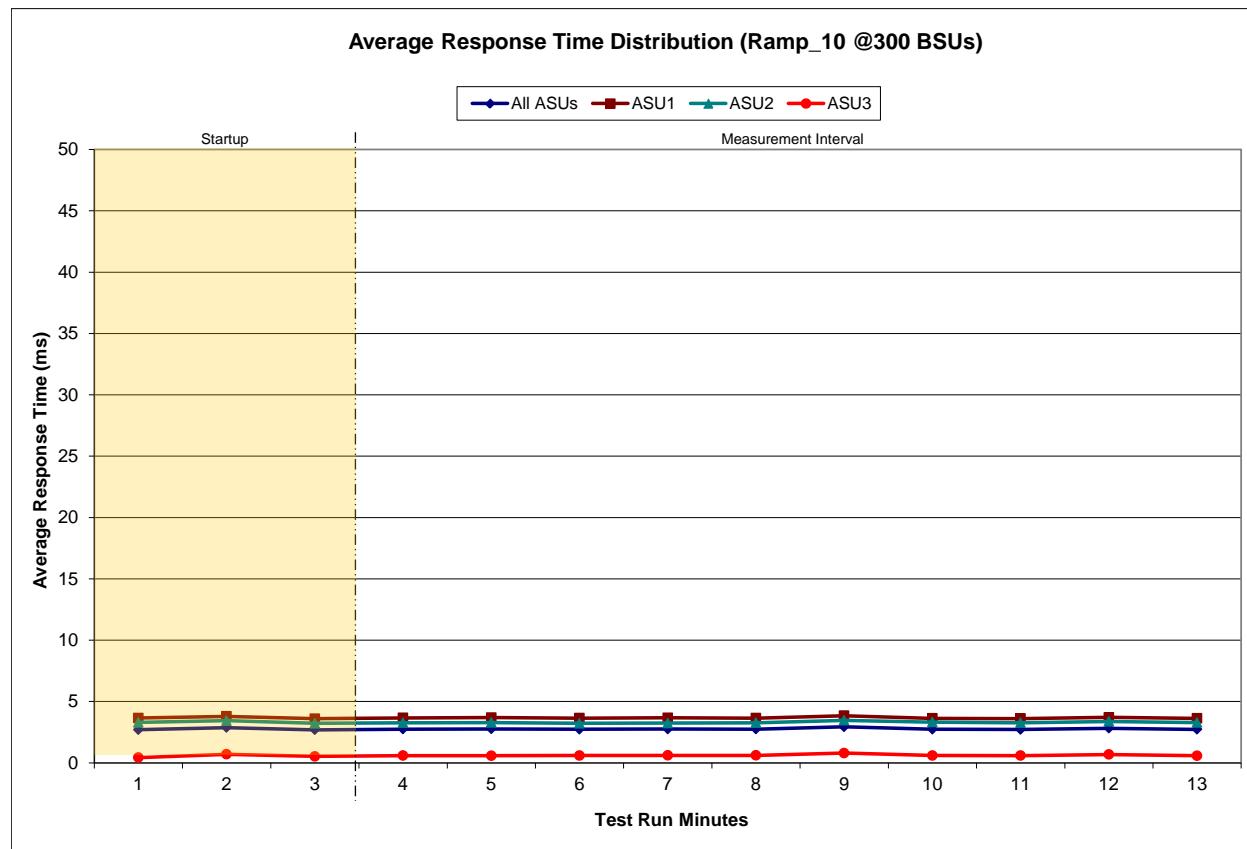

SPC-1 LRT™ (10%) – Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.15.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.15.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0701	0.2100	0.0180	0.0699	0.0351	0.2810
COV	0.006	0.002	0.005	0.003	0.007	0.003	0.006	0.001

Repeatability Test

Clause 5.4.5

The Repeatability Test demonstrates the repeatability and reproducibility of the SPC-1 IOPS™ primary metric and the SPC-1 LRT™ metric generated in earlier Test Runs.

There are two identical Repeatability Test Phases. Each Test Phase contains two Test Runs. Each of the Test Runs will have a Measurement Interval of no less than ten (10) minutes. The two Test Runs in each Test Phase will be executed without interruption or any type of manual intervention.

The first Test Run in each Test Phase is executed at the 10% load point. The Average Response Time from each of the Test Runs is compared to the SPC-1 LRT™ metric. Each Average Response Time value must be less than the SPC-1 LRT™ metric plus 5% or less than the SPC-1 LRT™ metric plus one (1) millisecond (ms).

The second Test Run in each Test Phase is executed at the 100% load point. The I/O Request Throughput from the Test Runs is compared to the SPC-1 IOPS™ primary metric. Each I/O Request Throughput value must be greater than the SPC-1 IOPS™ primary metric minus 5%. In addition, the Average Response Time for each Test Run cannot exceed 30 milliseconds.

If any of the above constraints are not met, the benchmark measurement is invalid.

Clause 9.4.3.7.4

The following content shall appear in the FDR for each Test Run in the two Repeatability Test Phases:

1. *A table containing the results of the Repeatability Test.*
2. *An I/O Request Throughput Distribution graph and table.*
3. *An Average Response Time Distribution graph and table.*
4. *The human readable Test Run Results File produced by the Workload Generator.*
5. *A listing or screen image of all input parameters supplied to the Workload Generator.*

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 72.

Repeatability Test Results File

The values for the SPC-1 IOPS™, SPC-1 LRT™, and the Repeatability Test measurements are listed in the tables below.

	SPC-1 IOPS™
Primary Metrics	150,286.25
Repeatability Test Phase 1	150,235.28
Repeatability Test Phase 2	150,275.09

The SPC-1 IOPS™ values in the above table were generated using 100% of the specified Business Scaling Unit (BSU) load level. Each of the Repeatability Test Phase values for SPC-1 IOPS™ must greater than 95% of the reported SPC-1 IOPS™ Primary Metric.

	SPC-1 LRT™
Primary Metrics	2.77 ms
Repeatability Test Phase 1	2.75 ms
Repeatability Test Phase 2	2.69 ms

The average response time values in the SPC-1 LRT™ column were generated using 10% of the specified Business Scaling Unit (BSU) load level. Each of the Repeatability Test Phase values for SPC-1 LRT™ must be less than 105% of the reported SPC-1 LRT™ Primary Metric or less than the reported SPC-1 LRT™ Primary Metric minus one (1) millisecond (ms).


A link to the test result file generated from each Repeatability Test Run is listed below.

- [Repeatability Test Phase 1, Test Run 1 \(LRT\)](#)
- [Repeatability Test Phase 1, Test Run 2 \(IOPS\)](#)
- [Repeatability Test Phase 2, Test Run 1 \(LRT\)](#)
- [Repeatability Test Phase 2, Test Run 2 \(IOPS\)](#)

Repeatability 1 LRT – I/O Request Throughput Distribution Data

300 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	21:13:50	21:16:50	0-2	0:03:00
Measurement Interval	21:16:50	21:26:50	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	15,002.77	8,937.40	1,838.95	4,226.42
1	15,009.03	8,947.32	1,838.63	4,223.08
2	14,999.03	8,927.97	1,845.13	4,225.93
3	14,983.80	8,938.47	1,838.57	4,206.77
4	15,006.17	8,949.65	1,848.23	4,208.28
5	14,998.38	8,942.17	1,848.72	4,207.50
6	14,993.17	8,940.75	1,841.12	4,211.30
7	14,977.58	8,916.35	1,844.57	4,216.67
8	14,966.43	8,916.28	1,844.78	4,205.37
9	14,997.65	8,943.82	1,839.37	4,214.47
10	14,975.60	8,918.92	1,841.45	4,215.23
11	14,988.90	8,932.43	1,846.30	4,210.17
12	15,006.13	8,932.07	1,854.63	4,219.43
Average	14,989.38	8,933.09	1,844.77	4,211.52


Repeatability 1 LRT – I/O Request Throughput Distribution Graph

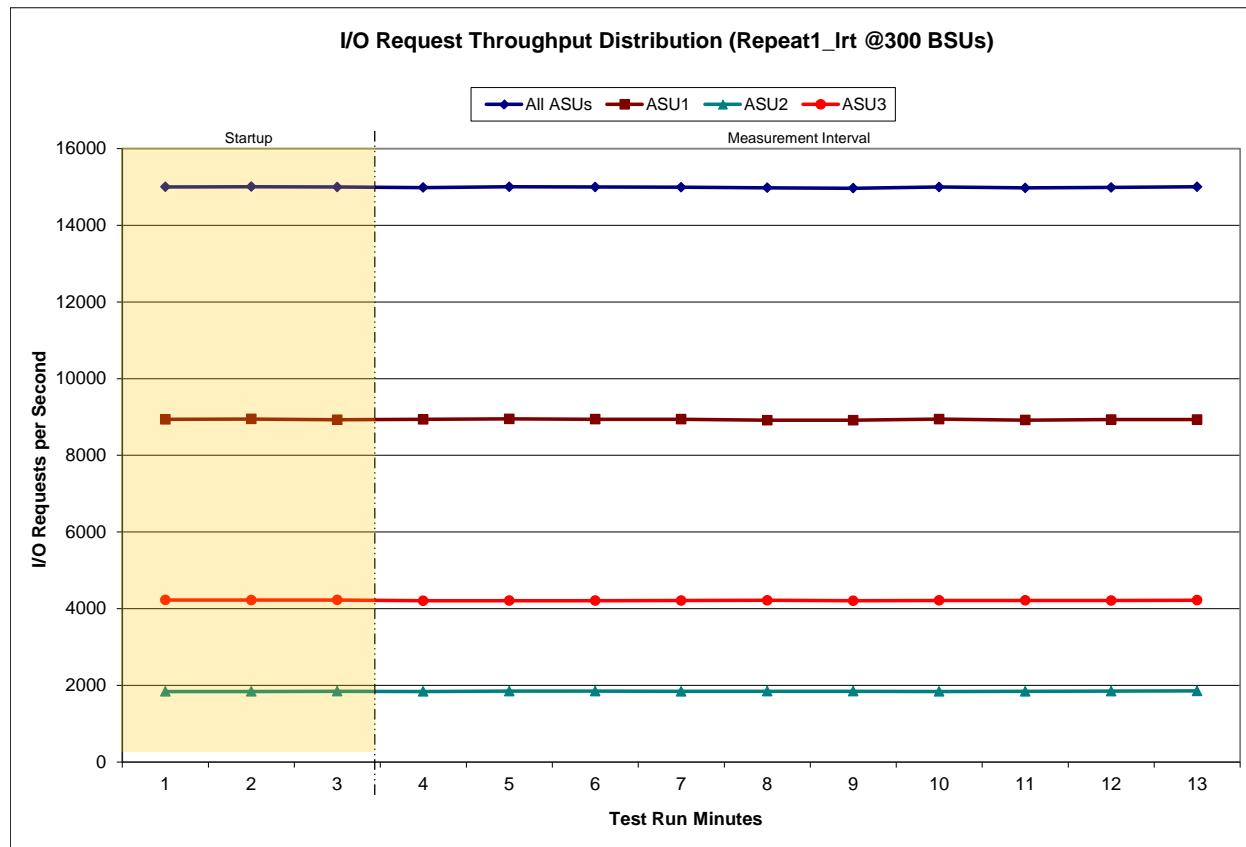

Repeatability 1 LRT –Average Response Time (ms) Distribution Data

300 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	21:13:50	21:16:50	0-2	0:03:00
Measurement Interval	21:16:50	21:26:50	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	2.88	3.81	3.46	0.67
1	2.75	3.65	3.31	0.62
2	2.75	3.65	3.32	0.59
3	2.75	3.64	3.31	0.59
4	2.75	3.65	3.27	0.60
5	2.76	3.65	3.32	0.60
6	2.73	3.63	3.29	0.59
7	2.72	3.61	3.29	0.59
8	2.72	3.61	3.30	0.58
9	2.74	3.64	3.30	0.60
10	2.90	3.80	3.46	0.77
11	2.72	3.61	3.25	0.60
12	2.71	3.60	3.26	0.59
Average	2.75	3.64	3.30	0.61


Repeatability 1 LRT –Average Response Time (ms) Distribution Graph

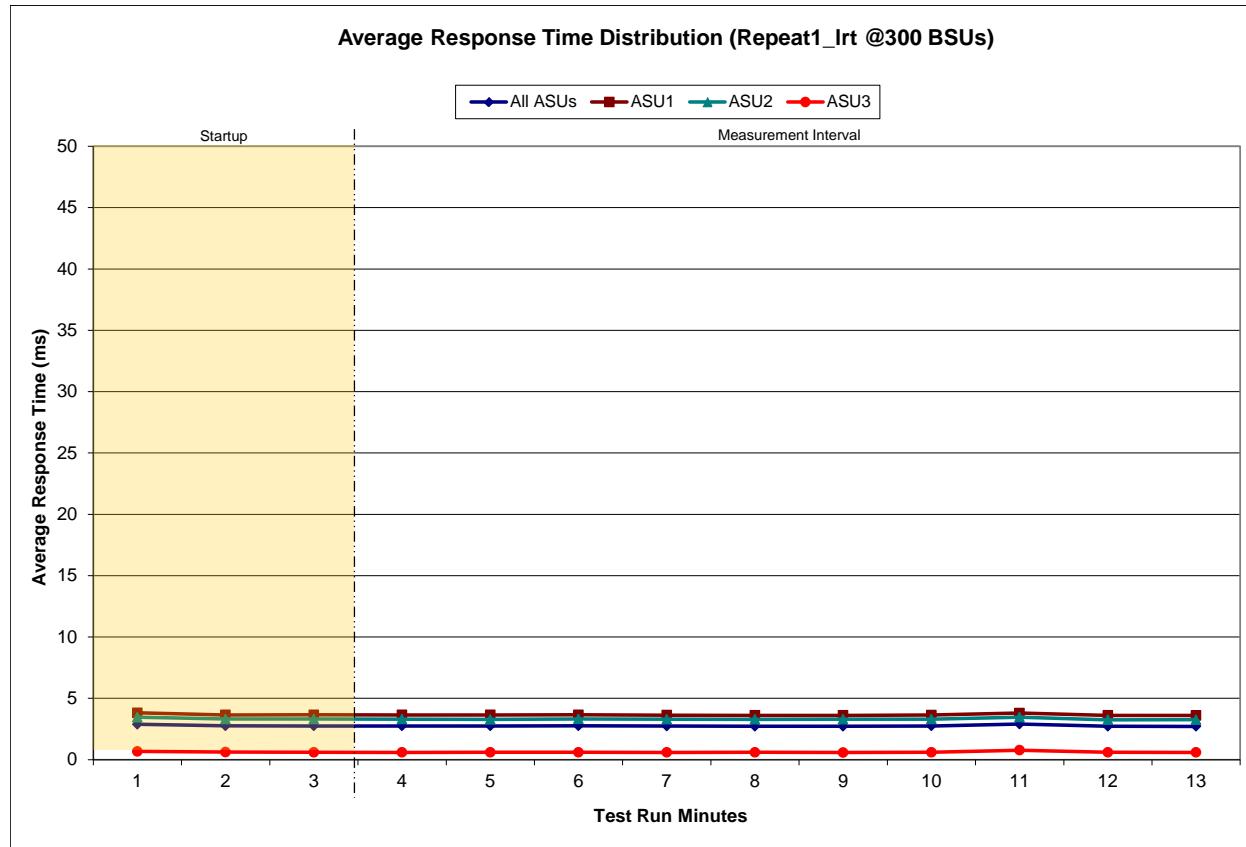

Repeatability 1 IOPS – I/O Request Throughput Distribution Data

3005 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	21:27:31	21:30:32	0-2	0:03:01
Measurement Interval	21:30:32	21:40:32	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	150,327.95	89,577.80	18,498.67	42,251.48
1	150,288.22	89,526.98	18,526.13	42,235.10
2	150,272.35	89,597.83	18,490.68	42,183.83
3	150,300.60	89,565.88	18,472.57	42,262.15
4	150,229.98	89,503.27	18,479.07	42,247.65
5	150,249.32	89,505.00	18,494.62	42,249.70
6	150,215.60	89,528.98	18,471.47	42,215.15
7	150,195.67	89,538.42	18,487.83	42,169.42
8	150,273.97	89,603.38	18,459.57	42,211.02
9	150,179.22	89,562.95	18,452.22	42,164.05
10	150,248.13	89,549.23	18,461.87	42,237.03
11	150,184.53	89,494.05	18,490.62	42,199.87
12	150,275.78	89,589.08	18,468.27	42,218.43
Average	150,235.28	89,544.03	18,473.81	42,217.45


Repeatability 1 IOPS – I/O Request Throughput Distribution Graph

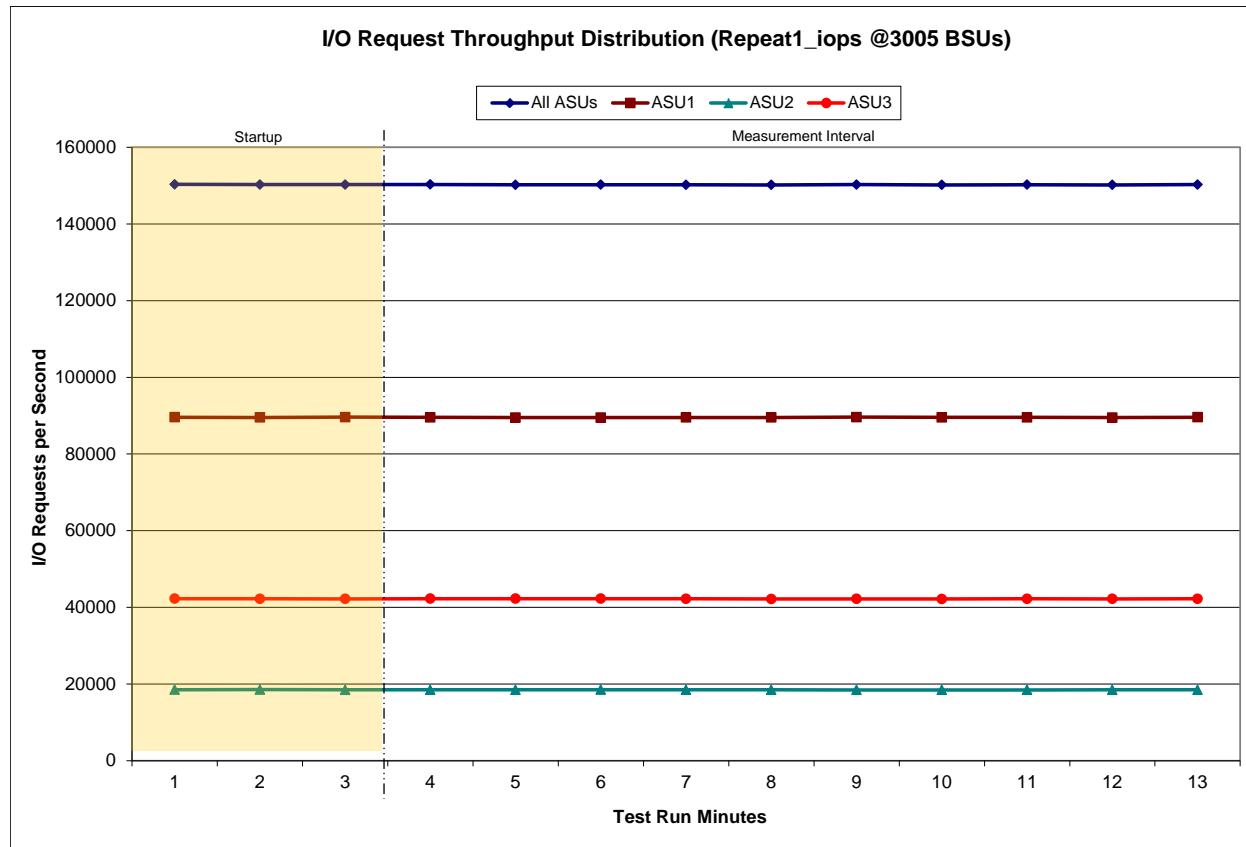

Repeatability 1 IOPS –Average Response Time (ms) Distribution Data

3005 BSUs	Start	Stop	Interval	Duration
<i>Start-Up/Ramp-Up</i>	21:27:31	21:30:32	0-2	0:03:01
<i>Measurement Interval</i>	21:30:32	21:40:32	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	8.70	10.53	15.58	1.79
1	7.51	9.14	12.91	1.68
2	7.36	9.08	12.11	1.63
3	7.23	8.86	12.24	1.58
4	7.32	8.96	12.28	1.67
5	7.32	9.01	12.08	1.64
6	7.31	8.97	12.23	1.62
7	7.41	9.09	12.26	1.71
8	7.23	8.90	12.12	1.54
9	7.28	8.90	12.36	1.62
10	7.39	9.07	11.97	1.84
11	7.31	8.94	12.33	1.63
12	7.34	9.03	12.08	1.67
Average	7.31	8.97	12.20	1.65


Repeatability 1 IOPS –Average Response Time (ms) Distribution Graph

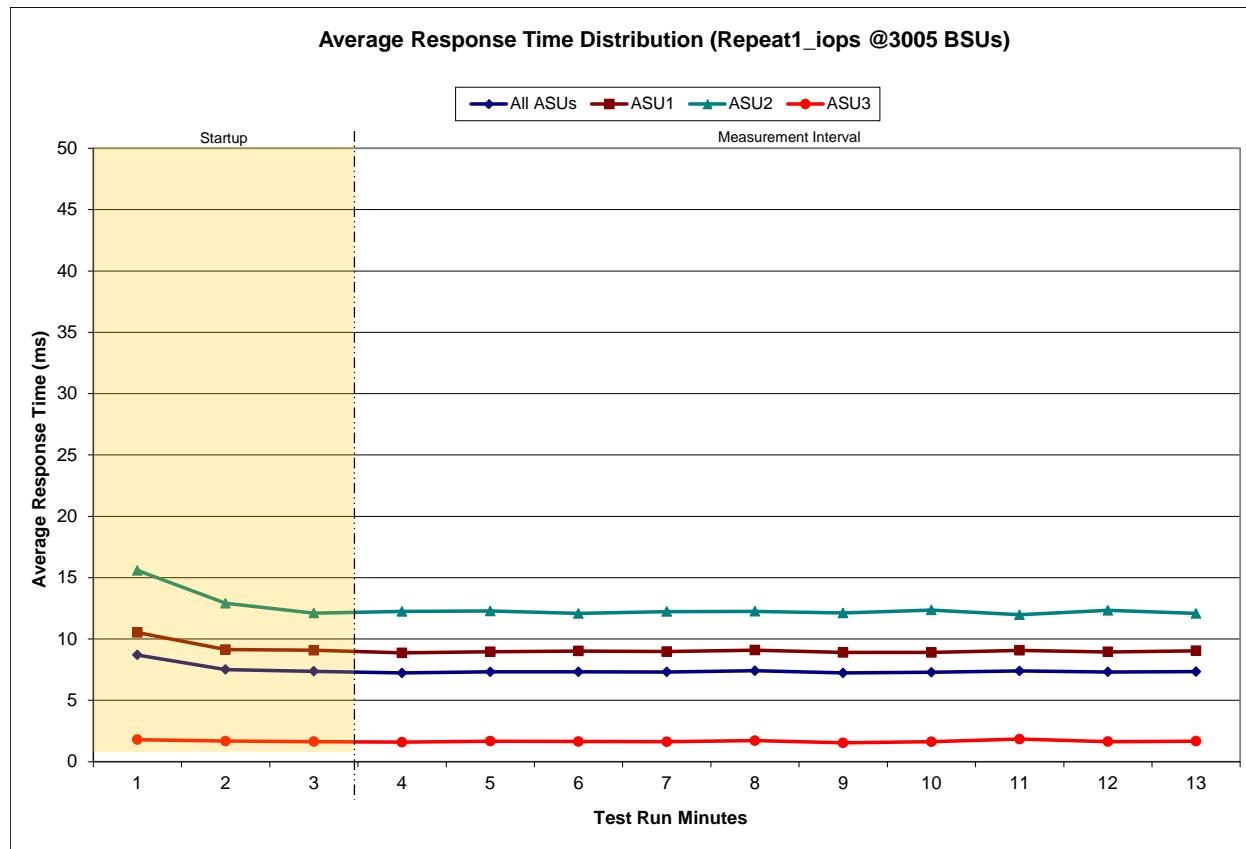

Repeatability 2 LRT – I/O Request Throughput Distribution Data

300 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	21:41:10	21:44:10	0-2	0:03:00
Measurement Interval	21:44:10	21:54:10	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	14,979.38	8,918.35	1,841.27	4,219.77
1	14,993.43	8,936.85	1,838.43	4,218.15
2	15,005.20	8,936.25	1,850.75	4,218.20
3	15,011.37	8,944.28	1,853.85	4,213.23
4	15,009.22	8,927.95	1,854.57	4,226.70
5	15,011.07	8,948.58	1,853.82	4,208.67
6	15,017.58	8,948.93	1,856.83	4,211.82
7	14,996.13	8,929.88	1,845.45	4,220.80
8	14,993.52	8,930.80	1,844.45	4,218.27
9	15,017.57	8,947.43	1,847.15	4,222.98
10	14,994.28	8,948.20	1,838.92	4,207.17
11	14,990.90	8,935.53	1,844.68	4,210.68
12	14,994.60	8,930.85	1,844.42	4,219.33
Average	15,003.62	8,939.25	1,848.41	4,215.97


Repeatability 2 LRT – I/O Request Throughput Distribution Graph

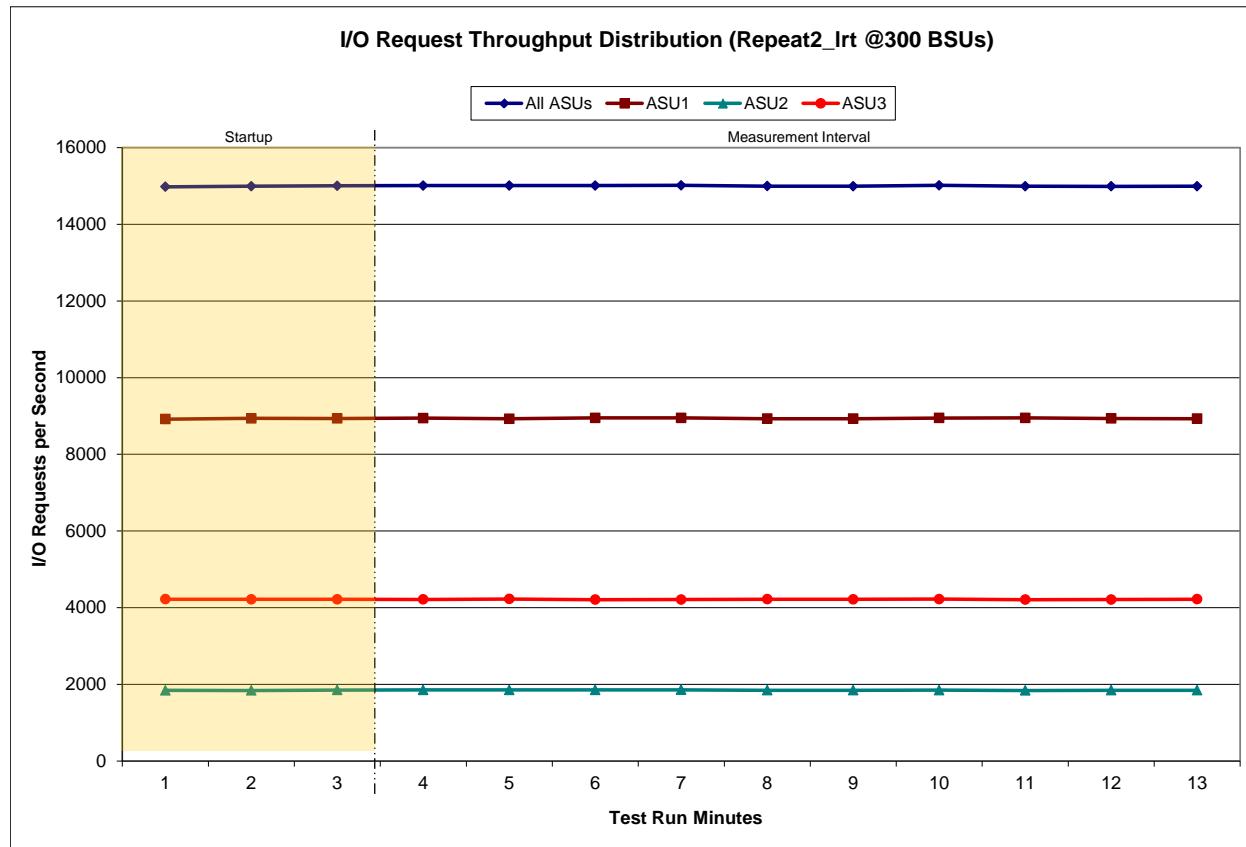

Repeatability 2 LRT –Average Response Time (ms) Distribution Data

300 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	21:41:10	21:44:10	0-2	0:03:00
Measurement Interval	21:44:10	21:54:10	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	2.99	3.95	3.60	0.70
1	2.67	3.60	3.28	0.43
2	2.64	3.56	3.22	0.43
3	2.63	3.54	3.20	0.44
4	2.69	3.60	3.27	0.52
5	2.67	3.57	3.25	0.51
6	2.65	3.54	3.22	0.50
7	2.67	3.56	3.26	0.53
8	2.69	3.57	3.24	0.59
9	2.73	3.62	3.25	0.61
10	2.73	3.62	3.28	0.61
11	2.73	3.62	3.26	0.60
12	2.71	3.61	3.23	0.60
Average	2.69	3.59	3.25	0.55


Repeatability 2 LRT –Average Response Time (ms) Distribution Graph

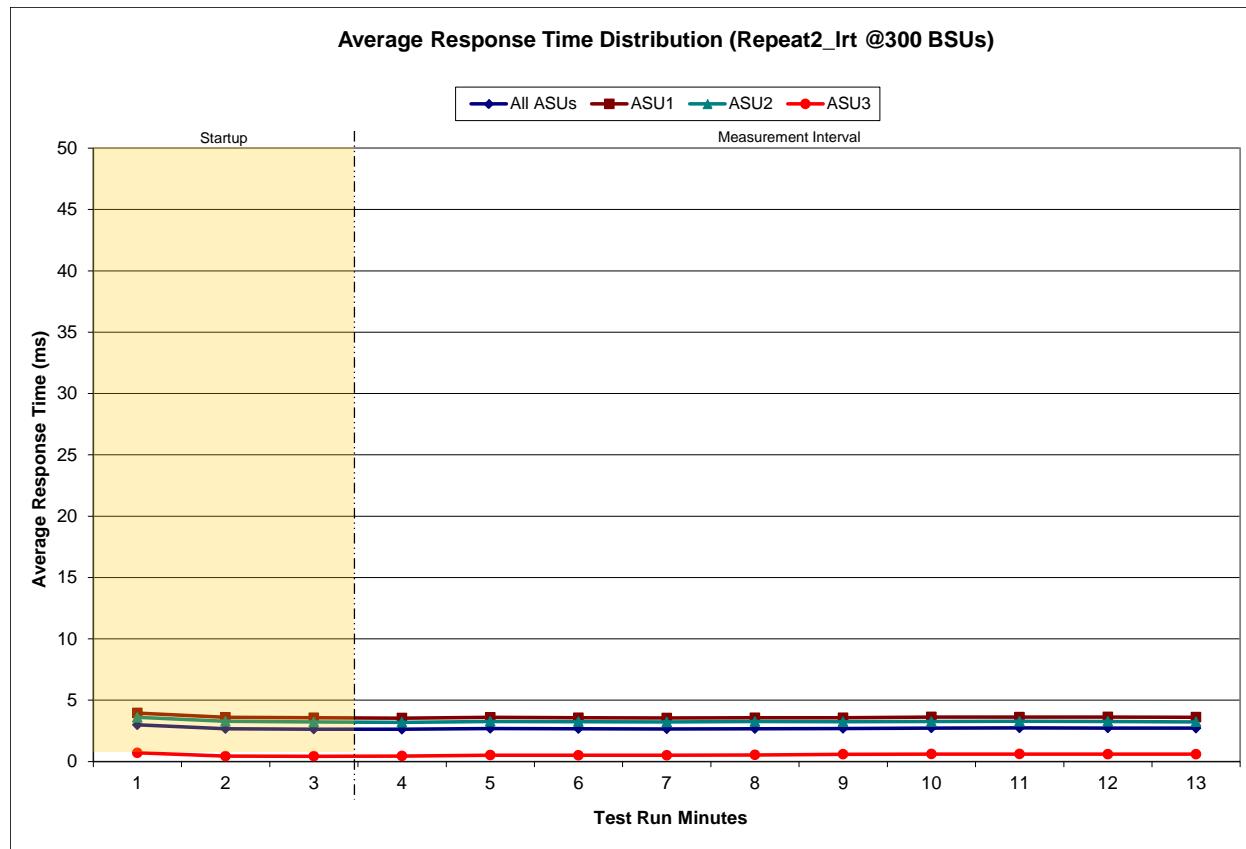

Repeatability 2 IOPS – I/O Request Throughput Distribution Data

3005 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	21:54:51	21:57:52	0-2	0:03:01
Measurement Interval	21:57:52	22:07:52	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	150,406.07	89,661.38	18,508.85	42,235.83
1	150,276.12	89,536.08	18,517.93	42,222.10
2	150,292.85	89,622.57	18,459.75	42,210.53
3	150,270.62	89,560.70	18,472.95	42,236.97
4	150,296.95	89,558.25	18,478.17	42,260.53
5	150,343.32	89,587.77	18,469.68	42,285.87
6	150,319.10	89,604.75	18,488.83	42,225.52
7	150,304.78	89,581.77	18,480.20	42,242.82
8	150,225.75	89,553.30	18,487.93	42,184.52
9	150,270.85	89,549.27	18,486.03	42,235.55
10	150,219.17	89,511.82	18,456.15	42,251.20
11	150,293.28	89,596.87	18,469.58	42,226.83
12	150,207.07	89,480.07	18,480.57	42,246.43
Average	150,275.09	89,558.46	18,477.01	42,239.62


Repeatability 2 IOPS – I/O Request Throughput Distribution Graph

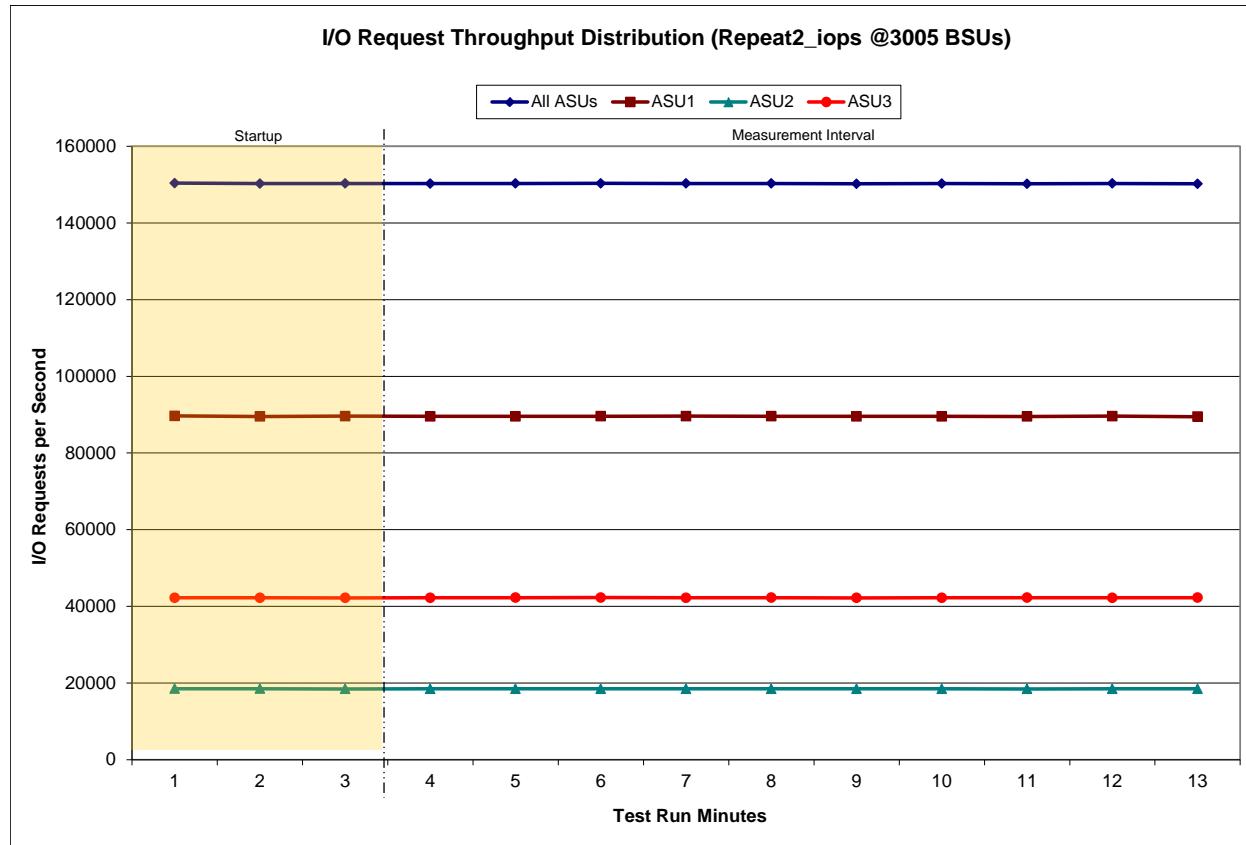

Repeatability 2 IOPS –Average Response Time (ms) Distribution Data

3005 BSUs	Start	Stop	Interval	Duration
Start-Up/Ramp-Up	21:54:51	21:57:52	0-2	0:03:01
Measurement Interval	21:57:52	22:07:52	3-12	0:10:00
60 second intervals	All ASUs	ASU1	ASU2	ASU3
0	8.69	10.46	15.77	1.82
1	7.45	9.19	12.32	1.61
2	7.30	8.88	12.58	1.66
3	7.41	9.14	12.03	1.70
4	7.27	8.86	12.42	1.64
5	7.28	8.98	11.90	1.65
6	7.33	8.98	12.26	1.65
7	7.27	8.92	12.30	1.56
8	7.33	9.02	12.13	1.62
9	7.34	8.97	12.39	1.66
10	7.32	9.01	12.12	1.64
11	7.31	8.95	12.35	1.62
12	7.29	8.97	12.08	1.61
Average	7.31	8.98	12.20	1.64

Repeatability 2 IOPS –Average Response Time (ms) Distribution Graph

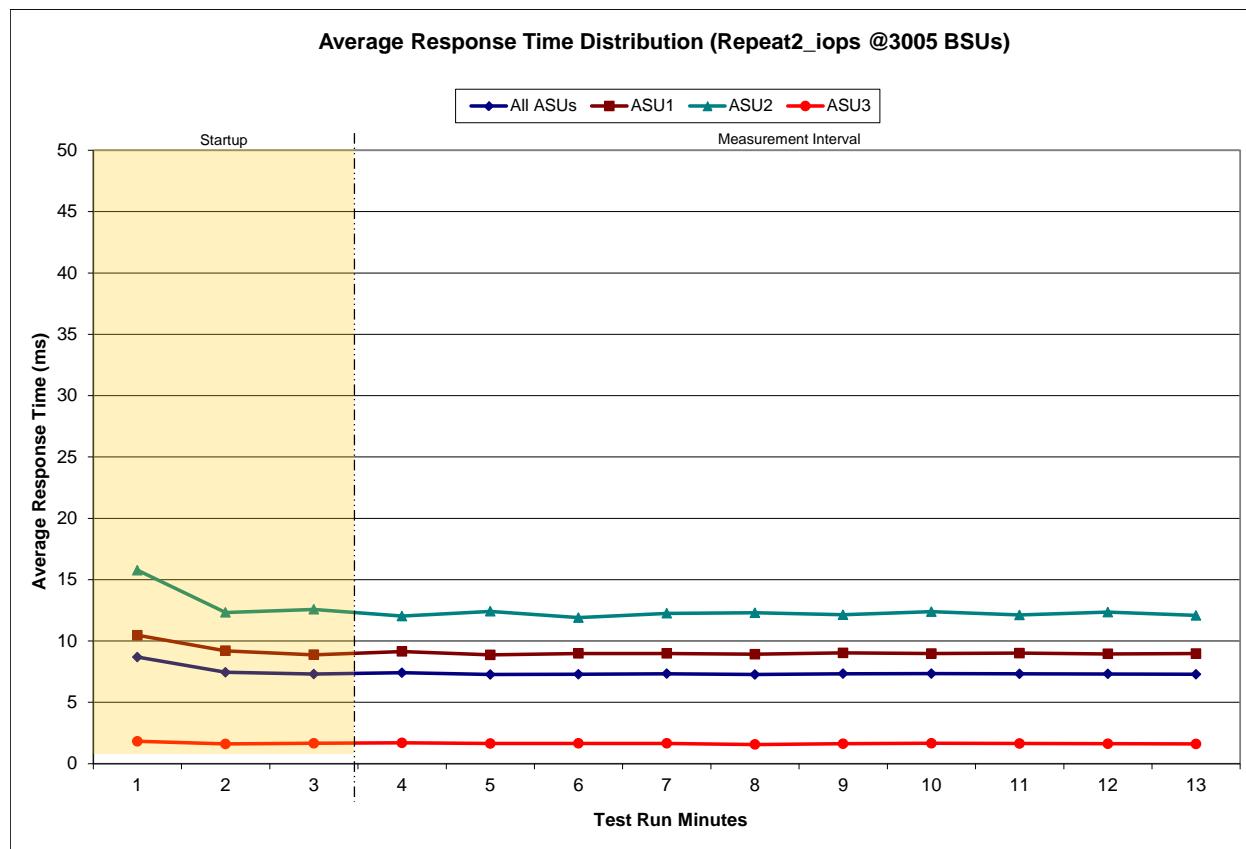

Repeatability 1 (LRT)

Measured Intensity Multiplier and Coefficient of Variation

Clause 3.4.3

IM – Intensity Multiplier: The ratio of I/Os for each I/O stream relative to the total I/Os for all I/O streams (ASU1-1 – ASU3-1) as required by the benchmark specification.

Clauses 5.1.10 and 5.3.15.2

MIM – Measured Intensity Multiplier: The Measured Intensity Multiplier represents the ratio of measured I/Os for each I/O stream relative to the total I/Os measured for all I/O streams (ASU1-1 – ASU3-1). This value may differ from the corresponding Expected Intensity Multiplier by no more than 5%.

Clause 5.3.15.3

COV – Coefficient of Variation: This measure of variation for the Measured Intensity Multiplier cannot exceed 0.2.

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
COV	0.002	0.002	0.006	0.003	0.008	0.004	0.004	0.001

Repeatability 1 (IOPS)

Measured Intensity Multiplier and Coefficient of Variation

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2811	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
COV	0.002	0.001	0.001	0.001	0.003	0.001	0.002	0.001

Repeatability 2 (LRT)

Measured Intensity Multiplier and Coefficient of Variation

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
IM	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0349	0.2810	0.0701	0.2098	0.0181	0.0701	0.0350	0.2810
COV	0.004	0.002	0.005	0.002	0.005	0.004	0.003	0.002

Repeatability 2 (IOPS)
Measured Intensity Multiplier and Coefficient of Variation

	ASU1-1	ASU1-2	ASU1-3	ASU1-4	ASU2-1	ASU2-2	ASU2-3	ASU3-1
<i>IM</i>	0.0350	0.2810	0.0700	0.2100	0.0180	0.0700	0.0350	0.2810
MIM	0.0350	0.2810	0.0700	0.2099	0.0180	0.0700	0.0350	0.2811
COV	0.001	0.000	0.001	0.001	0.002	0.001	0.001	0.001

Data Persistence Test

Clause 6

The Data Persistence Test demonstrates the Tested Storage Configuration (TSC):

- Is capable of maintaining data integrity across a power cycle.
- Ensures the transfer of data between Logical Volumes and host systems occurs without corruption or loss.

The SPC-1 Workload Generator will write 16 block I/O requests at random over the total Addressable Storage Capacity of the TSC for ten (10) minutes at a minimum of 25% of the load used to generate the SPC-1 IOPSTM primary metric. The bit pattern selected to be written to each block as well as the address of the block will be retained in a log file.

The Tested Storage Configuration (TSC) will be shutdown and restarted using a power off/power on cycle at the end of the above sequence of write operations. In addition, any caches employing battery backup must be flushed/emptied.

The SPC-1 Workload Generator will then use the above log file to verify each block written contains the correct bit pattern.

Clause 9.4.3.8

The following content shall appear in this section of the FDR:

1. A listing or screen image of all input parameters supplied to the Workload Generator.
2. For the successful Data Persistence Test Run, a table illustrating key results. The content, appearance, and format of this table are specified in Table 9-12. Information displayed in this table shall be obtained from the Test Run Results File referenced below in #3.
3. For the successful Data Persistence Test Run, the human readable Test Run Results file produced by the Workload Generator (may be contained in an appendix).

SPC-1 Workload Generator Input Parameters

The SPC-1 Workload Generator input parameters for the Sustainability, IOPS, Response Time Ramp, Repeatability, and Persistence Test Runs are documented in “Appendix E: SPC-1 Workload Generator Input Parameters” on Page 72.

Data Persistence Test Results File

A link to each test result file generated from each Data Persistence Test is listed below.

[Persistence 1 Test Results File](#)

[Persistence 2 Test Results File](#)

Data Persistence Test Results

Data Persistence Test Results	
Data Persistence Test Run Number: 1	
Total Number of Logical Blocks Written	270,207,152
Total Number of Logical Blocks Verified	161,128,784
Total Number of Logical Blocks that Failed Verification	0
Time Duration for Writing Test Logical Blocks	10 minutes
Size in bytes of each Logical Block	512
Number of Failed I/O Requests in the process of the Test	0

In some cases the same address was the target of multiple writes, which resulted in more Logical Blocks Written than Logical Blocks Verified. In the case of multiple writes to the same address, the pattern written and verified must be associated with the last write to that address.

PRICED STORAGE CONFIGURATION AVAILABILITY DATE

Clause 9.4.3.9

The committed delivery date for general availability (Availability Date) of all products that comprise the Priced Storage Configuration must be reported. When the Priced Storage Configuration includes products or components with different availability dates, the reported Availability Date for the Priced Storage Configuration must be the date at which all components are committed to be available.

The Huawei OceanStor™ S5800T as documented in this Full Disclosure Report is currently available for customer purchase and shipment.

PRICING INFORMATION

Clause 9.4.3.3.6

The Executive Summary shall contain a pricing spreadsheet as documented in Clause 8.3.1.

Pricing information may be found in the Priced Storage Configuration Pricing section on page 14.

TESTED STORAGE CONFIGURATION (TSC) AND PRICED STORAGE CONFIGURATION DIFFERENCES

Clause 9.4.3.3.8

The Executive Summary shall contain a list of all differences between the Tested Storage Configuration (TSC) and the Priced Storage Configuration.

A list of all differences between the Tested Storage Configuration (TSC) and Priced Storage Configuration may be found in the Executive Summary portion of this document on page 14.

ANOMALIES OR IRREGULARITIES

Clause 9.4.3.10

The FDR shall include a clear and complete description of any anomalies or irregularities encountered in the course of executing the SPC-1 benchmark that may in any way call into question the accuracy, verifiability, or authenticity of information published in this FDR.

There were no anomalies or irregularities encountered during the SPC-1 Remote Audit of the Huawei OceanStor™ S5800T.

APPENDIX A: SPC-1 GLOSSARY

“Decimal” (*powers of ten*) Measurement Units

In the storage industry, the terms “kilo”, “mega”, “giga”, “tera”, “peta”, and “exa” are commonly used prefixes for computing performance and capacity. For the purposes of the SPC workload definitions, all of the following terms are defined in “powers of ten” measurement units.

A kilobyte (KB) is equal to 1,000 (10^3) bytes.

A megabyte (MB) is equal to 1,000,000 (10^6) bytes.

A gigabyte (GB) is equal to 1,000,000,000 (10^9) bytes.

A terabyte (TB) is equal to 1,000,000,000,000 (10^{12}) bytes.

A petabyte (PB) is equal to 1,000,000,000,000,000 (10^{15}) bytes

An exabyte (EB) is equal to 1,000,000,000,000,000,000 (10^{18}) bytes

“Binary” (*powers of two*) Measurement Units

The sizes reported by many operating system components use “powers of two” measurement units rather than “power of ten” units. The following standardized definitions and terms are also valid and may be used in this document.

A kibibyte (KiB) is equal to 1,024 (2^{10}) bytes.

A mebibyte (MiB) is equal to 1,048,576 (2^{20}) bytes.

A gigabyte (GiB) is equal to 1,073,741,824 (2^{30}) bytes.

A tebibyte (TiB) is equal to 1,099,511,627,776 (2^{40}) bytes.

A pebibyte (PiB) is equal to 1,125,899,906,842,624 (2^{50}) bytes.

An exbibyte (EiB) is equal to 1,152,921,504,606,846,967 (2^{60}) bytes.

SPC-1 Data Repository Definitions

Total ASU Capacity: The total storage capacity read and written in the course of executing the SPC-1 benchmark.

Application Storage Unit (ASU): The logical interface between the storage and SPC-1 Workload Generator. The three ASUs (Data, User, and Log) are typically implemented on one or more Logical Volume.

Logical Volume: The division of Addressable Storage Capacity into individually addressable logical units of storage used in the SPC-1 benchmark. Each Logical Volume is implemented as a single, contiguous address space.

Addressable Storage Capacity: The total storage (sum of Logical Volumes) that can be read and written by application programs such as the SPC-1 Workload Generator.

Configured Storage Capacity: This capacity includes the Addressable Storage Capacity and any other storage (parity disks, hot spares, etc.) necessary to implement the Addressable Storage Capacity.

Physical Storage Capacity: The formatted capacity of all storage devices physically present in the Tested Storage Configuration (TSC).

Data Protection Overhead: The storage capacity required to implement the selected level of data protection.

Required Storage: The amount of Configured Storage Capacity required to implement the Addressable Storage Configuration, excluding the storage required for the three ASUs.

Global Storage Overhead: The amount of Physical Storage Capacity that is required for storage subsystem use and unavailable for use by application programs.

Total Unused Storage: The amount of storage capacity available for use by application programs but not included in the Total ASU Capacity.

SPC-1 Data Protection Levels

Protected 1: The single point of failure of any *storage device* in the configuration will not result in permanent loss of access to or integrity of the SPC-1 Data Repository.

Protected 2: The single point of failure of any *component* in the configuration will not result in permanent loss of access to or integrity of the SPC-1 Data Repository.

SPC-1 Test Execution Definitions

Average Response Time: The sum of the Response Times for all Measured I/O Requests divided by the total number of Measured I/O Requests.

Completed I/O Request: An I/O Request with a Start Time and a Completion Time (see “I/O Completion Types” below).

Completion Time: The time recorded by the Workload Generator when an I/O Request is satisfied by the TSC as signaled by System Software.

Data Rate: The data transferred in all Measured I/O Requests in an SPC-1 Test Run divided by the length of the Test Run in seconds.

Expected I/O Count: For any given I/O Stream and Test Phase, the product of 50 times the BSU level, the duration of the Test Phase in seconds, and the Intensity Multiplier for that I/O Stream.

Failed I/O Request: Any I/O Request issued by the Workload Generator that could not be completed or was signaled as failed by System Software. A Failed I/O Request has no Completion Time (see “I/O Completion Types” below).

I/O Request Throughput: The total number of Measured I/O requests in an SPC-1 Test Run divided by the duration of the Measurement Interval in seconds.

In-Flight I/O Request: An I/O Request issued by the I/O Command Generator to the TSC that has a recorded Start Time, but does not complete within the Measurement Interval (see “I/O Completion Types” below).

Measured I/O Request: A Completed I/O Request with a Completion Time occurring within the Measurement Interval (see “I/O Completion Types” below).

Measured Intensity Multiplier: The percentage of all Measured I/O Requests that were issued by a given I/O Stream.

Measurement Interval: The finite and contiguous time period, after the TSC has reached Steady State, when data is collected by a Test Sponsor to generate an SPC-1 test result or support an SPC-1 test result.

Ramp-Up: The time required for the Benchmark Configuration (BC) to produce Steady State throughput after the Workload Generator begins submitting I/O Requests to the TSC for execution.

Ramp-Down: The time required for the BC to complete all I/O Requests issued by the Workload Generator. The Ramp-Down period begins when the Workload Generator ceases to issue new I/O Requests to the TSC.

Response Time: The Response Time of a Measured I/O Request is its Completion Time minus its Start Time.

Start Time: The time recorded by the Workload Generator when an I/O Request is submitted, by the Workload Generator, to the System Software for execution on the Tested Storage Configuration (TSC).

Start-Up: The period that begins after the Workload Generator starts to submit I/O requests to the TSC and ends at the beginning of the Measurement Interval.

Shut-Down: The period between the end of the Measurement Interval and the time when all I/O Requests issued by the Workload Generator have completed or failed.


Steady State: The consistent and sustainable throughput of the TSC. During this period the load presented to the TSC by the Workload Generator is constant.

Test: A collection of Test Phases and or Test Runs sharing a common objective.


Test Run: The execution of SPC-1 for the purpose of producing or supporting an SPC-1 test result. SPC-1 Test Runs may have a finite and measured Ramp-Up period, Start-Up period, Shut-Down period, and Ramp-Down period as illustrated in the “SPC-1 Test Run Components” below. All SPC-1 Test Runs shall have a Steady State period and a Measurement Interval.

Test Phase: A collection of one or more SPC-1 Test Runs sharing a common objective and intended to be run in a specific sequence.

I/O Completion Types

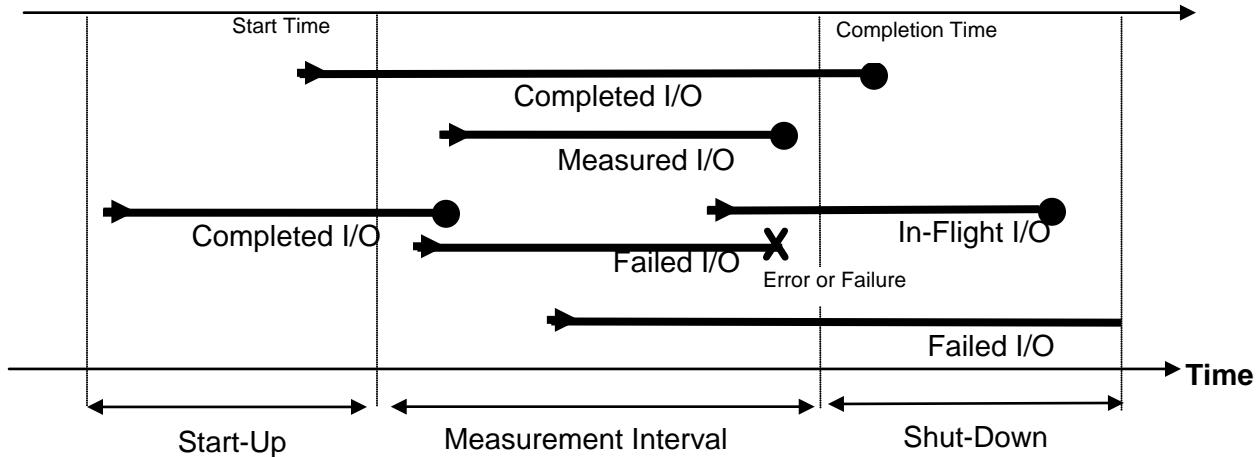

SPC-1 Test Run Components

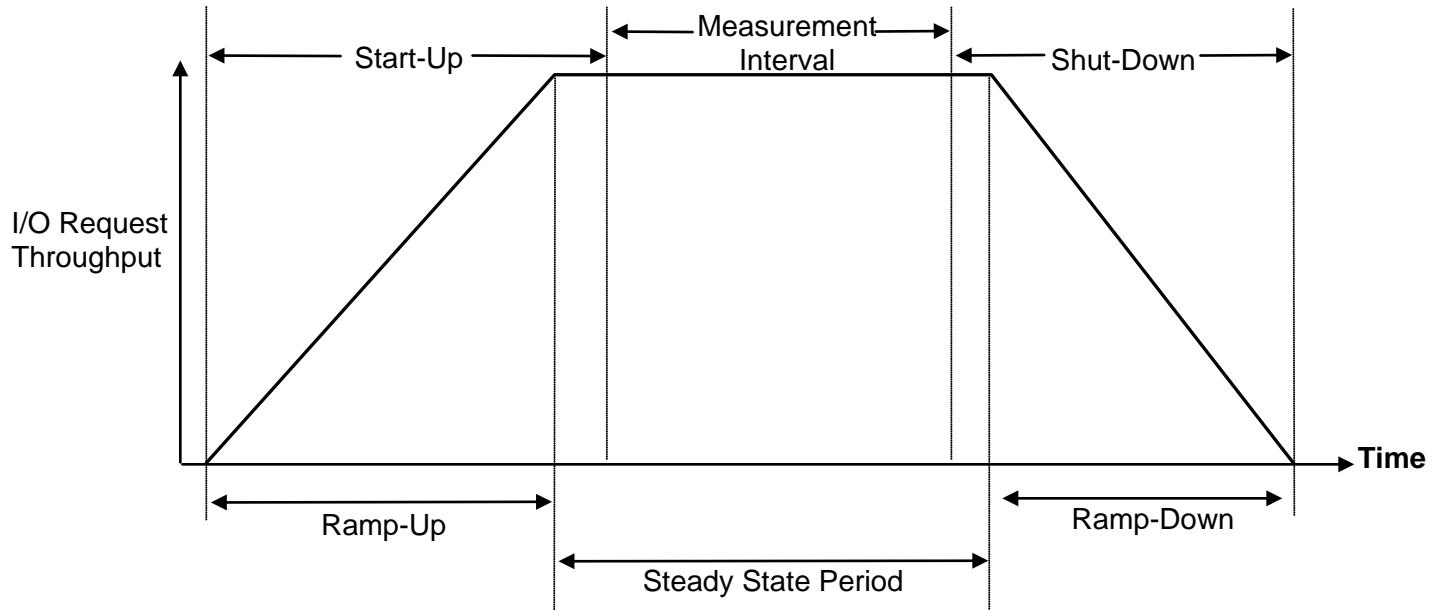

APPENDIX B: CUSTOMER TUNABLE PARAMETERS AND OPTIONS

Red Hat Enterprise Linux 5.5 (64-bit)

Change the I/O scheduler from ***cfq*** to ***noop*** on each Host System, which will result in all incoming I/O requests inserted into a simple, unordered FIFO queue. This was done by execution of the [***scheduler.sh***](#) script as documented in “*Appendix C: Tested Storage Configuration (TSC) Creation*”.

APPENDIX C: TESTED STORAGE CONFIGURATION (TSC) CREATION

Step 1 Create Host Group and Host

Execute the following commands in OceanStor S5800T's CLI to create one host group *HostGroup001*, and add *Host001* and *Host002* to the host group, then add 4 host FC ports WWNs to *Host001* and add the other 4 FC ports WWNs to *Host002*.

The **-t** parameter is used in the command **addhost** to define the host operating system type, and **-t 0** means Linux. The **-type** parameter of command **addhostport** means port type, and **type 1** means FC host port.

```
createhostgroup -n HostGroup001
addhost -group 1 -n Host001 -t 0
addhost -group 1 -n Host002 -t 0
addhostport -host 0 -type 1 -wwn 21000024ff2087b6 -n FCInitiator001
addhostport -host 0 -type 1 -wwn 21000024ff2087b7 -n FCInitiator002
addhostport -host 0 -type 1 -wwn 21000024ff2088e2 -n FCInitiator003
addhostport -host 0 -type 1 -wwn 21000024ff2088e3 -n FCInitiator004
addhostport -host 1 -type 1 -wwn 21000024ff2c9498 -n FCInitiator005
addhostport -host 1 -type 1 -wwn 21000024ff28ea72 -n FCInitiator006
addhostport -host 1 -type 1 -wwn 21000024ff2c9499 -n FCInitiator007
addhostport -host 1 -type 1 -wwn 21000024ff28ea73 -n FCInitiator008
```

Step 2 Create RAID Groups and LUNs


Execute the [**mklun.sh**](#) script on the Host System, which has **expect** installed. The script will create 34 RAID Groups, 34 LUNs (*one LUN per RAID Group*) and map the LUNs to *HostGroup001*.

Note: Expect is a Unix automation and testing tool, written by Don Libes as an extension to the Tcl scripting language, for interactive applications such as telnet, ftp, passwd, fsck, rlogin, tip, ssh, and others. It uses Unix pseudo terminals to wrap up subprocesses transparently, allowing the automation of arbitrary applications that are accessed over a terminal. Expect is an open source tool can be downloaded at the following location: <http://www.nist.gov/el/msid/expect.cfm>

The **createlun** commands create one LUN per RAID Group and use all of the available capacity for the LUN. The **addhostmap** command maps a LUN to a host or a host group.

RAID Groups 0-31 each contain six 300 GB disk drives. Four of the disk drives in RAID Group 0 are vault disk drives, each of which as 23 GiB reserved to store “dirty” data in case of a power failure. RAID Groups 32 and 33 each contain six 600 GB disk drives.

The RAID-Disk mapping is illustrated below.

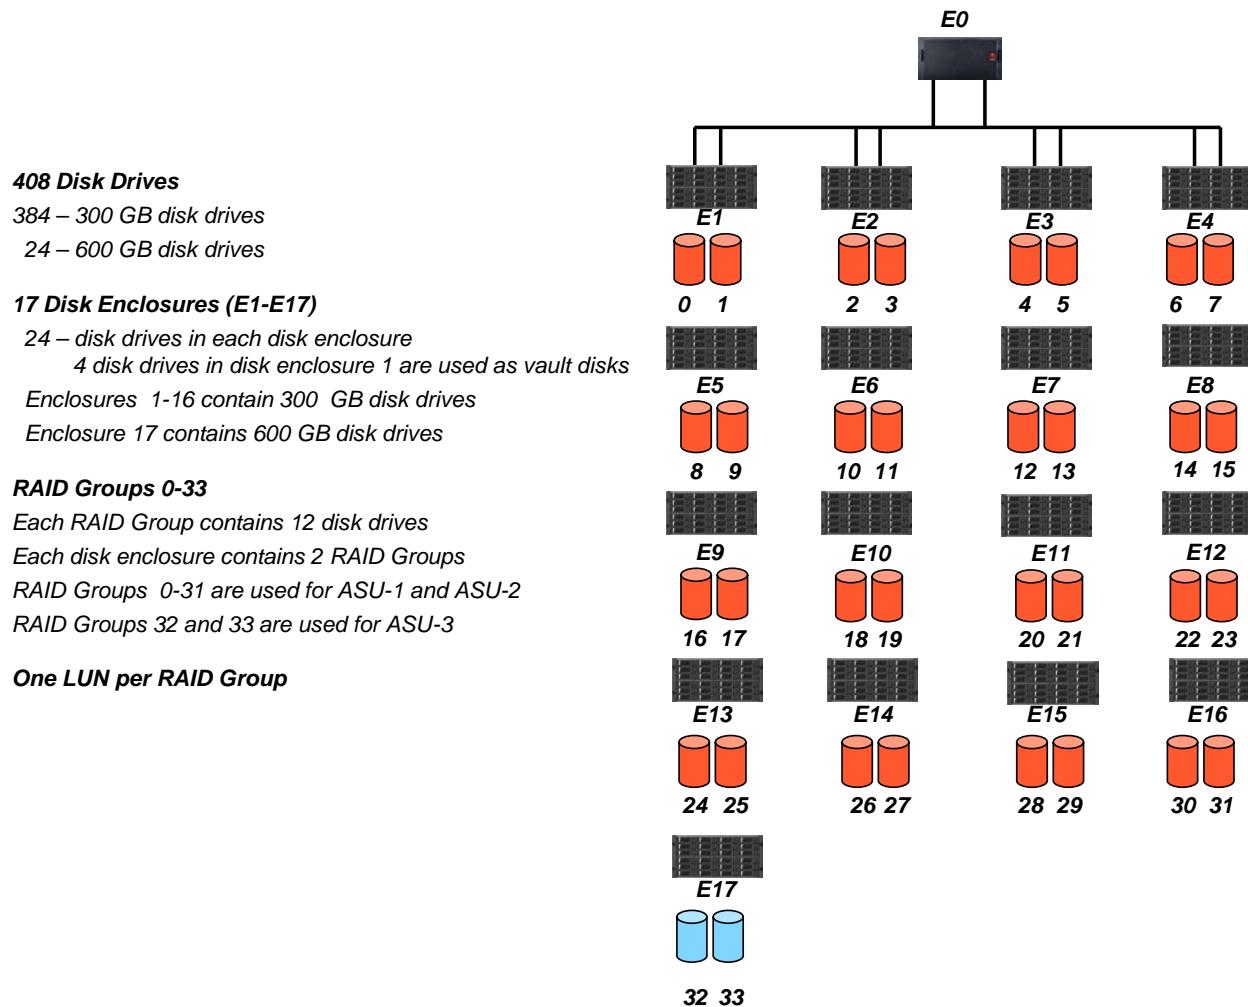

Step 3 Change the low and high water level of storage

Execute the following command, using the OceanStor S5800T's CLI to change the low water level to 40 and the high water level to 50.

```
chgcachewaterlevel -low 40
chgcachewaterlevel -high 50
```

Step 4 Create Volumes on the Host System

Execute the [mkvolume.sh](#) script on the Host System to create 44 logical volumes.

1. Create Physical Volumes

Invoke **pvccreate** on each block device, creating 34 physical volumes

2. Create Volume Groups

Create **vg0** using: /dev/sdc, /dev/sdd, /dev/sde, /dev/sdf, /dev/sdg, /dev/sdh, /dev/sdi, /dev/sdj, /dev/sdk, /dev/sdl, /dev/sdm, /dev/sdn, /dev/sdo, /dev/sdp, /dev/sdq, /dev/sdr, /dev/sds, /dev/sdt, /dev/sdu, /dev/sdv, /dev/sdw, /dev/sdx, /dev/sdy, /dev/sdz, /dev/sdaa, /dev/sdab, /dev/sdac, /dev/sdad, /dev/sdae, /dev/sdaf, /dev/sdag, /dev/sdah

Create **vg1** using: /dev/sdai, /dev/sdaj

3. Create Logical Volumes

- Create 20 logical volumes on vg0 for ASU-1, each with a capacity of 1,057.5 GiB.
- Create 20 logical volumes on vg0 for ASU-2, each with a capacity of 1,057.5 GiB.
- Create 4 logical volumes on vg1 for ASU-3, each with a capacity of 1,175 GiB.

4. Scan Logical Volumes

Scan the logical volumes on the second Host System.

Step 5 Change the schedule on each block device

Execute the [**scheduler.sh**](#) script on each Host System to change the scheduler of each block device from **cfq** to **noop**.

Referenced Scripts

mklun.sh

```
#!/bin/bash

stor=129.27.228.169
stor_user=admin
stor_pswd=Admin@storage

export LANG=C

echo "creating LUN ..."

expect << __END_CREATE_LUN
    spawn ssh $stor_user@$stor
    expect {
        "assword" {
            send "$stor_pswd\r"
        }
        "yes/no" {
            send "yes\r"
            expect "assword"
            send "$stor_pswd\r"
        }
    }
    expect ">"

    set timeout 60

    set lunid 0
```

```

set rgid 0

foreach enclosure {1: 2: 3: 4: 5: 6: 7: 8: 9: 10: 11: 12: 13: 14: 15: 16: 17: }
{
    foreach diskset {0,1,2,3,4,5,6,7,8,9,10,11
12,13,14,15,16,17,18,19,20,21,22,23} {
        set disk_list ""
        foreach disk [split \$diskset ,] {
            set list_unit [string map [list : ,\$disk:] \$enclosure]
            append disk_list \$list_unit
        }
        send "createrg -n ASU-\$rgid -l 10 -num 2 -list \$disk_list\r"
        expect {
            "(y/n)" {
                send "y\r"
            }
            ">" {
                send "\r"
            }
        }
        expect ">"
        send "showrg -rg \$rgid\r"
        expect ">"
        if [ expr \$lunid%2 ] {
            set ctrl b
        } else {
            set ctrl a
        }
        if { \$lunid >= 12 && \$lunid <= 41 } {
            send "createlun -rg \$rgid -n ASU-\$lunid -susize 512 -
pretype 1 -value 4 -c \$ctrl\r"
        } else {
            send "createlun -rg \$rgid -n ASU-\$lunid -susize 512 -pretype 0
-c \$ctrl\r"
        }
        expect ">"
        sleep 1
        send "showlun -lun \$lunid\r"
        expect ">"
        send "addhostmap -group 1 -devlun \$lunid\r"
        expect ">"
        send "showhostmap -map [expr \$lunid + 1048576]\r"
        expect ">"
        incr lunid
        incr rgid
    }
}
send "exit\r"
expect "(y/n):"
send "y\r"
expect EOF
__END_CREATE_LUN

```

mkvolume.sh

```
pvcreate /dev/sdc
pvcreate /dev/sdd
pvcreate /dev/sde
pvcreate /dev/sdf
pvcreate /dev/sdg
pvcreate /dev/sdh
pvcreate /dev/sdi
pvcreate /dev/sdj
pvcreate /dev/sdk
pvcreate /dev/sdl
pvcreate /dev/sdm
pvcreate /dev/sdn
pvcreate /dev/sdo
pvcreate /dev/sdp
pvcreate /dev/sdq
pvcreate /dev/sdr
pvcreate /dev/sds
pvcreate /dev/sdt
pvcreate /dev/sdu
pvcreate /dev/sdv
pvcreate /dev/sdw
pvcreate /dev/sdx
pvcreate /dev/sdy
pvcreate /dev/sdz
pvcreate /dev/sdaa
pvcreate /dev/sdab
pvcreate /dev/sdac
pvcreate /dev/sdad
pvcreate /dev/sdae
pvcreate /dev/sdaf
pvcreate /dev/sdag
pvcreate /dev/sdah
pvcreate /dev/sdai
pvcreate /dev/sdaj

vgcreate vg0 /dev/sdc /dev/sdd /dev/sde /dev/sdf /dev/sdg /dev/sdh /dev/sdi /dev/sdj
/dev/sdk /dev/sdl /dev/sdm /dev/sdn /dev/sdo /dev/sdp /dev/sdq /dev/sdr /dev/sds
/dev/sdt /dev/sdu /dev/sdv /dev/sdw /dev/sdx /dev/sdy /dev/sdz /dev/sdaa /dev/sdab
/dev/sdac /dev/sdad /dev/sdae /dev/sdaf /dev/sdag /dev/sdah
vgcreate vgl /dev/sdai /dev/sdaj

lvcreate -n asul11 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul12 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul13 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul14 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul15 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul16 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul17 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul18 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul19 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul10 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul11 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul12 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul13 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul14 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul15 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul16 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul17 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asul18 -i 32 -I 512 -L 1057.5g vg0
```

```
lvcreate -n asu119 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu120 -i 32 -I 512 -L 1057.5g vg0

lvcreate -n asu21 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu22 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu23 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu24 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu25 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu26 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu27 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu28 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu29 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu210 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu211 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu212 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu213 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu214 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu215 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu216 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu217 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu218 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu219 -i 32 -I 512 -L 1057.5g vg0
lvcreate -n asu220 -i 32 -I 512 -L 1057.5g vg0

lvcreate -n asu31 -i 2 -I 512 -L 1175g vg1
lvcreate -n asu32 -i 2 -I 512 -L 1175g vg1
lvcreate -n asu33 -i 2 -I 512 -L 1175g vg1
lvcreate -n asu34 -i 2 -I 512 -L 1175g vg1

for host in host1
121 do
122 ssh $host pvscan
123 ssh $host vgscan
124 ssh $host lvscan
125 ssh $host lvchange -ay /dev/vg0/asu11
126 ssh $host lvchange -ay /dev/vg0/asu12
127 ssh $host lvchange -ay /dev/vg0/asu13
128 ssh $host lvchange -ay /dev/vg0/asu14
129 ssh $host lvchange -ay /dev/vg0/asu15
130 ssh $host lvchange -ay /dev/vg0/asu16
131 ssh $host lvchange -ay /dev/vg0/asu17
132 ssh $host lvchange -ay /dev/vg0/asu18
133 ssh $host lvchange -ay /dev/vg0/asu19
134 ssh $host lvchange -ay /dev/vg0/asu110
135 ssh $host lvchange -ay /dev/vg0/asu111
136 ssh $host lvchange -ay /dev/vg0/asu112
137 ssh $host lvchange -ay /dev/vg0/asu113
138 ssh $host lvchange -ay /dev/vg0/asu114
139 ssh $host lvchange -ay /dev/vg0/asu115
140 ssh $host lvchange -ay /dev/vg0/asu116
141 ssh $host lvchange -ay /dev/vg0/asu117
142 ssh $host lvchange -ay /dev/vg0/asu118
143 ssh $host lvchange -ay /dev/vg0/asu119
144 ssh $host lvchange -ay /dev/vg0/asu120
145
146 ssh $host lvchange -ay /dev/vg0/asu21
147 ssh $host lvchange -ay /dev/vg0/asu22
148 ssh $host lvchange -ay /dev/vg0/asu23
149 ssh $host lvchange -ay /dev/vg0/asu24
150 ssh $host lvchange -ay /dev/vg0/asu25
151 ssh $host lvchange -ay /dev/vg0/asu26
152 ssh $host lvchange -ay /dev/vg0/asu27
153 ssh $host lvchange -ay /dev/vg0/asu28
```

```
154 ssh $host lvchange -ay /dev/vg0/asu29
155 ssh $host lvchange -ay /dev/vg0/asu210
156 ssh $host lvchange -ay /dev/vg0/asu211
157 ssh $host lvchange -ay /dev/vg0/asu212
158 ssh $host lvchange -ay /dev/vg0/asu213
159 ssh $host lvchange -ay /dev/vg0/asu214
160 ssh $host lvchange -ay /dev/vg0/asu215
161 ssh $host lvchange -ay /dev/vg0/asu216
162 ssh $host lvchange -ay /dev/vg0/asu217
163 ssh $host lvchange -ay /dev/vg0/asu218
164 ssh $host lvchange -ay /dev/vg0/asu219
165 ssh $host lvchange -ay /dev/vg0/asu220
166
167 ssh $host lvchange -ay /dev/vg1/asu31
168 ssh $host lvchange -ay /dev/vg1/asu32
169 ssh $host lvchange -ay /dev/vg1/asu33
170 ssh $host lvchange -ay /dev/vg1/asu34
173 done
```

scheduler.sh

```
echo noop > /sys/block/sdc/queue/scheduler
echo noop > /sys/block/sdd/queue/scheduler
echo noop > /sys/block/sde/queue/scheduler
echo noop > /sys/block/sdf/queue/scheduler
echo noop > /sys/block/sdg/queue/scheduler
echo noop > /sys/block/sdh/queue/scheduler
echo noop > /sys/block/sdi/queue/scheduler
echo noop > /sys/block/sdj/queue/scheduler
echo noop > /sys/block/sdk/queue/scheduler
echo noop > /sys/block/sdl/queue/scheduler
echo noop > /sys/block/sdm/queue/scheduler
echo noop > /sys/block/sdn/queue/scheduler
echo noop > /sys/block/sdo/queue/scheduler
echo noop > /sys/block/sdp/queue/scheduler
echo noop > /sys/block/sdq/queue/scheduler
echo noop > /sys/block/sdr/queue/scheduler
echo noop > /sys/block/sds/queue/scheduler
echo noop > /sys/block/sdt/queue/scheduler
echo noop > /sys/block/sdu/queue/scheduler
echo noop > /sys/block/sdv/queue/scheduler
echo noop > /sys/block/sdw/queue/scheduler
echo noop > /sys/block/sdx/queue/scheduler
echo noop > /sys/block/sdy/queue/scheduler
echo noop > /sys/block/sdz/queue/scheduler
echo noop > /sys/block/sdaa/queue/scheduler
echo noop > /sys/block/sdab/queue/scheduler
echo noop > /sys/block/sdac/queue/scheduler
echo noop > /sys/block/sdad/queue/scheduler
echo noop > /sys/block/sdae/queue/scheduler
echo noop > /sys/block/sdaf/queue/scheduler
echo noop > /sys/block/sdag/queue/scheduler
echo noop > /sys/block/sdah/queue/scheduler
echo noop > /sys/block/sdai/queue/scheduler
echo noop > /sys/block/sdaj/queue/scheduler
```

APPENDIX D: SPC-1 WORKLOAD GENERATOR STORAGE COMMANDS AND PARAMETERS

ASU Pre-Fill

The content of command and parameter file, used in this benchmark to execute the required ASU pre-fill, is listed below.

```
pattern=/root/S5800T/random
hd=default,vdbench=/root/vdbench,user=root,shell=ssh
hd=hd1,system=host1
hd=hd2,system=host2
sd=default,threads=1
sd=sd1,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu11,size=1135481978880
sd=sd2,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu12,size=1135481978880
sd=sd3,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu13,size=1135481978880
sd=sd4,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu14,size=1135481978880
sd=sd5,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu15,size=1135481978880
sd=sd6,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu16,size=1135481978880
sd=sd7,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu17,size=1135481978880
sd=sd8,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu18,size=1135481978880
sd=sd9,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu19,size=1135481978880
sd=sd10,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu110,size=1135481978880
sd=sd11,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu111,size=1135481978880
sd=sd12,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu112,size=1135481978880
sd=sd13,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu113,size=1135481978880
sd=sd14,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu114,size=1135481978880
sd=sd15,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu115,size=1135481978880
sd=sd16,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu116,size=1135481978880
sd=sd17,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu117,size=1135481978880
sd=sd18,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu118,size=1135481978880
sd=sd19,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu119,size=1135481978880
sd=sd20,hd=hd1,openflags=o_direct,lun=/dev/vg0/asu120,size=1135481978880
sd=sd21,hd=hd1,openflags=o_direct,lun=/dev/vg1/asu31,size=1261646643200
sd=sd22,hd=hd1,openflags=o_direct,lun=/dev/vg1/asu32,size=1261646643200
sd=sd23,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu21,size=1135481978880
sd=sd24,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu22,size=1135481978880
sd=sd25,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu23,size=1135481978880
sd=sd26,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu24,size=1135481978880
sd=sd27,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu25,size=1135481978880
sd=sd28,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu26,size=1135481978880
sd=sd29,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu27,size=1135481978880
sd=sd30,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu28,size=1135481978880
sd=sd31,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu29,size=1135481978880
sd=sd32,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu210,size=1135481978880
sd=sd33,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu211,size=1135481978880
sd=sd34,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu212,size=1135481978880
sd=sd35,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu213,size=1135481978880
sd=sd36,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu214,size=1135481978880
sd=sd37,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu215,size=1135481978880
sd=sd38,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu216,size=1135481978880
sd=sd39,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu217,size=1135481978880
sd=sd40,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu218,size=1135481978880
sd=sd41,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu219,size=1135481978880
sd=sd42,hd=hd2,openflags=o_direct,lun=/dev/vg0/asu220,size=1135481978880
sd=sd43,hd=hd2,openflags=o_direct,lun=/dev/vg1/asu33,size=1261646643200
sd=sd44,hd=hd2,openflags=o_direct,lun=/dev/vg1/asu34,size=1261646643200
wd=wd1,sd=sd*,rdpct=0,seekpct=-1,xfersize=512K
rd=PREPSSD,wd=wd1,iorate=max,elapsed=360000,interval=10
```

Primary Metrics and Repeatability Tests

The content of SPC-1 Workload Generator command and parameter file, used in this benchmark to execute the Primary Metrics and Repeatability Tests, is listed below.

```
host=master
slaves=(slave1,slave2,slave3,slave4,slave5,slave6,slave7,slave8,slave9,slave10,slave
11,slave12,slave13,slave14,slave15,slave16,slave17,slave18,slave19,slave20,slave21,s
lave22,slave23,slave24,slave25,slave26,slave27,slave28,slave29,slave30,slave31,slave
32,slave33,slave34,slave35,slave36,slave37,slave38,slave39,slave40)

sd=asu1_1,lun=/dev/vg0/asu11 ,size=1135481978880
sd=asu1_2,lun=/dev/vg0/asu12 ,size=1135481978880
sd=asu1_3,lun=/dev/vg0/asu13 ,size=1135481978880
sd=asu1_4,lun=/dev/vg0/asu14 ,size=1135481978880
sd=asu1_5,lun=/dev/vg0/asu15 ,size=1135481978880
sd=asu1_6,lun=/dev/vg0/asu16 ,size=1135481978880
sd=asu1_7,lun=/dev/vg0/asu17 ,size=1135481978880
sd=asu1_8,lun=/dev/vg0/asu18 ,size=1135481978880
sd=asu1_9,lun=/dev/vg0/asu19 ,size=1135481978880
sd=asu1_10,lun=/dev/vg0/asu110,size=1135481978880
sd=asu1_11,lun=/dev/vg0/asu111,size=1135481978880
sd=asu1_12,lun=/dev/vg0/asu112,size=1135481978880
sd=asu1_13,lun=/dev/vg0/asu113,size=1135481978880
sd=asu1_14,lun=/dev/vg0/asu114,size=1135481978880
sd=asu1_15,lun=/dev/vg0/asu115,size=1135481978880
sd=asu1_16,lun=/dev/vg0/asu116,size=1135481978880
sd=asu1_17,lun=/dev/vg0/asu117,size=1135481978880
sd=asu1_18,lun=/dev/vg0/asu118,size=1135481978880
sd=asu1_19,lun=/dev/vg0/asu119,size=1135481978880
sd=asu1_20,lun=/dev/vg0/asu120,size=1135481978880

sd=asu2_1,lun=/dev/vg0/asu21 ,size= 1135481978880
sd=asu2_2,lun=/dev/vg0/asu22 ,size= 1135481978880
sd=asu2_3,lun=/dev/vg0/asu23 ,size= 1135481978880
sd=asu2_4,lun=/dev/vg0/asu24 ,size= 1135481978880
sd=asu2_5,lun=/dev/vg0/asu25 ,size=1135481978880
sd=asu2_6,lun=/dev/vg0/asu26 ,size=1135481978880
sd=asu2_7,lun=/dev/vg0/asu27 ,size=1135481978880
sd=asu2_8,lun=/dev/vg0/asu28 ,size=1135481978880
sd=asu2_9,lun=/dev/vg0/asu29 ,size=1135481978880
sd=asu2_10,lun=/dev/vg0/asu210,size=1135481978880
sd=asu2_11,lun=/dev/vg0/asu211,size=1135481978880
sd=asu2_12,lun=/dev/vg0/asu212,size=1135481978880
sd=asu2_13,lun=/dev/vg0/asu213,size=1135481978880
sd=asu2_14,lun=/dev/vg0/asu214,size=1135481978880
sd=asu2_15,lun=/dev/vg0/asu215,size=1135481978880
sd=asu2_16,lun=/dev/vg0/asu216,size=1135481978880
sd=asu2_17,lun=/dev/vg0/asu217,size=1135481978880
sd=asu2_18,lun=/dev/vg0/asu218,size=1135481978880
sd=asu2_19,lun=/dev/vg0/asu219,size=1135481978880
sd=asu2_20,lun=/dev/vg0/asu220,size=1135481978880

sd=asu3_1,lun=/dev/vg1/asu31 ,size=1261646643200
sd=asu3_2,lun=/dev/vg1/asu32 ,size=1261646643200
sd=asu3_3,lun=/dev/vg1/asu33 ,size=1261646643200
sd=asu3_4,lun=/dev/vg1/asu34 ,size=1261646643200
```

SPC-1 Persistence Test

The content of SPC-1 Workload Generator command and parameter file, used in this benchmark to execute the SPC-1 Persistence Test, is listed below.

```
sd=asul_1,lun=/dev/vg0/asul1 ,size=1135481978880
sd=asul_2,lun=/dev/vg0/asul2 ,size=1135481978880
sd=asul_3,lun=/dev/vg0/asul3 ,size=1135481978880
sd=asul_4,lun=/dev/vg0/asul4 ,size=1135481978880
sd=asul_5,lun=/dev/vg0/asul5 ,size=1135481978880
sd=asul_6,lun=/dev/vg0/asul6 ,size=1135481978880
sd=asul_7,lun=/dev/vg0/asul7 ,size=1135481978880
sd=asul_8,lun=/dev/vg0/asul8 ,size=1135481978880
sd=asul_9,lun=/dev/vg0/asul9 ,size=1135481978880
sd=asul_10,lun=/dev/vg0/asul10 ,size=1135481978880
sd=asul_11,lun=/dev/vg0/asul11 ,size=1135481978880
sd=asul_12,lun=/dev/vg0/asul12 ,size=1135481978880
sd=asul_13,lun=/dev/vg0/asul13 ,size=1135481978880
sd=asul_14,lun=/dev/vg0/asul14 ,size=1135481978880
sd=asul_15,lun=/dev/vg0/asul15 ,size=1135481978880
sd=asul_16,lun=/dev/vg0/asul16 ,size=1135481978880
sd=asul_17,lun=/dev/vg0/asul17 ,size=1135481978880
sd=asul_18,lun=/dev/vg0/asul18 ,size=1135481978880
sd=asul_19,lun=/dev/vg0/asul19 ,size=1135481978880
sd=asul_20,lun=/dev/vg0/asul20 ,size=1135481978880

sd=asu2_1,lun=/dev/vg0/asu21 ,size= 1135481978880
sd=asu2_2,lun=/dev/vg0/asu22 ,size= 1135481978880
sd=asu2_3,lun=/dev/vg0/asu23 ,size= 1135481978880
sd=asu2_4,lun=/dev/vg0/asu24 ,size= 1135481978880
sd=asu2_5,lun=/dev/vg0/asu25 ,size=1135481978880
sd=asu2_6,lun=/dev/vg0/asu26 ,size=1135481978880
sd=asu2_7,lun=/dev/vg0/asu27 ,size=1135481978880
sd=asu2_8,lun=/dev/vg0/asu28 ,size=1135481978880
sd=asu2_9,lun=/dev/vg0/asu29 ,size=1135481978880
sd=asu2_10,lun=/dev/vg0/asu210 ,size=1135481978880
sd=asu2_11,lun=/dev/vg0/asu211 ,size=1135481978880
sd=asu2_12,lun=/dev/vg0/asu212 ,size=1135481978880
sd=asu2_13,lun=/dev/vg0/asu213 ,size=1135481978880
sd=asu2_14,lun=/dev/vg0/asu214 ,size=1135481978880
sd=asu2_15,lun=/dev/vg0/asu215 ,size=1135481978880
sd=asu2_16,lun=/dev/vg0/asu216 ,size=1135481978880
sd=asu2_17,lun=/dev/vg0/asu217 ,size=1135481978880
sd=asu2_18,lun=/dev/vg0/asu218 ,size=1135481978880
sd=asu2_19,lun=/dev/vg0/asu219 ,size=1135481978880
sd=asu2_20,lun=/dev/vg0/asu220 ,size=1135481978880

sd=asu3_1,lun=/dev/vg1/asu31 ,size=1261646643200
sd=asu3_2,lun=/dev/vg1/asu32 ,size=1261646643200
sd=asu3_3,lun=/dev/vg1/asu33 ,size=1261646643200
sd=asu3_4,lun=/dev/vg1/asu34 ,size=1261646643200
```

APPENDIX E: SPC-1 WORKLOAD GENERATOR INPUT PARAMETERS

ASU Pre-Fill, Primary Metrics Test, Repeatability Test, Persistence Test Run 1, TSC power off/power on and Persistence Test Run 2

The following script was used to execute the required ASU pre-fill, Primary Metrics Test (*Sustainability Test Phase, IOPS Test Phase, and Response Time Ramp Test Phase*), Repeatability Test (*Repeatability Test Phase 1 and Repeatability Test Phase 2*), and Persistence Test Run 1 in an uninterrupted sequence. The script pauses until the required TSC power off/power on cycle is completed then executes Persistence Test Run 2.

The script also included the appropriate commands to capture the detailed TSC profile listings required for a Remote Audit.

```
JAVA="/usr/java/jre1.7.0_06/bin/java -Xms4096m -Xmx4096m -Xss256k"
EXEDIR=/root/S5800T

expect shstorage.tcl > profile1_storage.log
date > profile1_volume.log
pvdisplay >> profile1_volume.log
vgdisplay >> profile1_volume.log
lvdisplay >> profile1_volume.log
date >> profile1_volume.log

..../vdbench/vdbench -f prefilling.cfg -o prefilling

N=1
for host in host2 host1
do
    ssh $host rm -rf $EXEDIR/output
    ssh $host rm -rf $EXEDIR/config
    ssh $host mkdir $EXEDIR/output
    ssh $host mkdir $EXEDIR/config
    for((i=1;i<=20;i++))
    do
        echo "start slave$N on $host"
        echo "master=host2" > $EXEDIR/config/slave$N.cfg
        echo "host=slave$N" >> $EXEDIR/config/slave$N.cfg

        echo "sd=asul_1,lun=/dev/vg0/asu11 ,size=1135481978880 " >>
$EXEDIR/config/slave$N.cfg
        echo "sd=asul_2,lun=/dev/vg0/asu12 ,size=1135481978880 " >>
$EXEDIR/config/slave$N.cfg
        echo "sd=asul_3,lun=/dev/vg0/asu13 ,size=1135481978880 " >>
$EXEDIR/config/slave$N.cfg
        echo "sd=asul_4,lun=/dev/vg0/asu14 ,size=1135481978880 " >>
$EXEDIR/config/slave$N.cfg
        echo "sd=asul_5,lun=/dev/vg0/asu15 ,size=1135481978880 " >>
$EXEDIR/config/slave$N.cfg
        echo "sd=asul_6,lun=/dev/vg0/asu16 ,size=1135481978880 " >>
$EXEDIR/config/slave$N.cfg
        echo "sd=asul_7,lun=/dev/vg0/asu17 ,size=1135481978880 " >>
$EXEDIR/config/slave$N.cfg
        echo "sd=asul_8,lun=/dev/vg0/asu18 ,size=1135481978880 " >>
$EXEDIR/config/slave$N.cfg
        echo "sd=asul_9,lun=/dev/vg0/asu19 ,size=1135481978880 " >>
$EXEDIR/config/slave$N.cfg
        echo "sd=asul_10,lun=/dev/vg0/asu110,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
```

```
echo "sd=asul_11,lun=/dev/vg0/asul11,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asul_12,lun=/dev/vg0/asul12,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asul_13,lun=/dev/vg0/asul13,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asul_14,lun=/dev/vg0/asul14,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asul_15,lun=/dev/vg0/asul15,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asul_16,lun=/dev/vg0/asul16,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asul_17,lun=/dev/vg0/asul17,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asul_18,lun=/dev/vg0/asul18,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asul_19,lun=/dev/vg0/asul19,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asul_20,lun=/dev/vg0/asul20,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg

echo "sd=asu2_1,lun=/dev/vg0/asu21 ,size= 1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_2,lun=/dev/vg0/asu22 ,size= 1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_3,lun=/dev/vg0/asu23 ,size= 1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_4,lun=/dev/vg0/asu24 ,size= 1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_5,lun=/dev/vg0/asu25 ,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_6,lun=/dev/vg0/asu26 ,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_7,lun=/dev/vg0/asu27 ,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_8,lun=/dev/vg0/asu28 ,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_9,lun=/dev/vg0/asu29 ,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_10,lun=/dev/vg0/asu210,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_11,lun=/dev/vg0/asu211,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_12,lun=/dev/vg0/asu212,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_13,lun=/dev/vg0/asu213,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_14,lun=/dev/vg0/asu214,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_15,lun=/dev/vg0/asu215,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_16,lun=/dev/vg0/asu216,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_17,lun=/dev/vg0/asu217,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_18,lun=/dev/vg0/asu218,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_19,lun=/dev/vg0/asu219,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu2_20,lun=/dev/vg0/asu220,size=1135481978880" >>
$EXEDIR/config/slave$N.cfg
```

```
echo "sd=asu3_1,lun=/dev/vg1/asu31 ,size=1261646643200" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu3_2,lun=/dev/vg1/asu32 ,size=1261646643200" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu3_3,lun=/dev/vg1/asu33 ,size=1261646643200" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu3_4,lun=/dev/vg1/asu34 ,size=1261646643200" >>
$EXEDIR/config/slave$N.cfg
echo "sd=asu3_6,lun=/dev/vg1/asu36 ,size=1261646643200" >>
$EXEDIR/config/slave$N.cfg

scp $EXEDIR/config/slave$N.cfg $host:$EXEDIR/config/slave$N.cfg
ssh $host "$JAVA -cp $EXEDIR/../spcl spcl -f $EXEDIR/config/slave$N.cfg -o
$EXEDIR/output/slave$N" > /dev/null &
N=$[N+1]
done
done

rm -rf spcl.cfg
cp metrics.cfg spcl.cfg

$JAVA -cp ../spcl metrics -b 3005 -t 28800
$JAVA -cp ../spcl repeat1 -b 3005
$JAVA -cp ../spcl repeat2 -b 3005

for host in host1 host2
do
    ssh $host killall java
done

rm -rf spcl.cfg
cp persist.cfg spcl.cfg

$JAVA -cp ../spcl persist1 -b 2255

echo "Power cycle TSC, then Enter to continue"
read

expect shstorage.tcl > profile2_storage.log
date > profile2_volume.log
pvdisplay >> profile2_volume.log
vgdisplay >> profile2_volume.log
lvdisplay >> profile2_volume.log
date >> profile2_volume.log

$JAVA -cp ../spcl persist2
```

APPENDIX F: THIRD-PARTY QUOTATION



Even Enterprises
12439 Magnolia Blvd. Suite# 303
N. Hollywood, CA 91607
Phone: 818-793-4403
Fax: 818-302-3344

Even Enterprises Quotation

Issued To:	«Company» «First_Name» «Last_Name» «City», «State»	DATE ISSUED:	November 12, 2012
Phone:	«Business_Phone»	PAYMENT TERMS:	Credit Card / Net 30 (upon approval)
Email:	«Email»	Salesperson:	Esti Even
		Prices subject to change without notice	
		Prices Valid for 90 days	Confidential

No.	Model	Description	Add	Unit Price (\$)	Total Price (\$)
1	Phase				295,522.00
1.1	Location				295,522.00
1.1.1	S5800T		1		295,522.00
1.1.1.1	Control module				43,757.00
	SPE61C0200-S56-2C96G-BASE	SPE61C0200-56 Controller Enclosure(Dual Controller,AC,96GB Cache,with UPS Cache Protected Module,without Front-End & Back-End Port,with HS Storage Array Control System Software)	1	43,757.00	43,757.00
1.1.1.2	Disk Enclosure				51,102.00
	DAE12435U4-AC	DAE12435U4-03 Disk Enclosure(4U,3.5",AC,SAS Expansion Module,without Disk Unit,with HS SAS in Band Management Software)	17	3,006.00	51,102.00
1.1.1.3	Hard Disk Drives				176,568.00
	SAS300-15K	300GB 15K RPM SAS Disk Unit(3.5")	384	418.00	160,512.00
	SAS600-15K	600GB 15K RPM SAS Disk Unit(3.5")	24	669.00	16,056.00
1.1.1.4	IO Interface				10,710.00
	LPU4F8	4*8Gbps Fibre Channel I/O modules(Total 4 ports)	2	1,219.00	2,438.00
	LPU2S6	2*24Gbps SAS-wide I/O modules(Total 2 ports)	8	1,034.00	8,272.00
1.1.1.5	Accessory				519.00
	SS-OP-D-LC-M-3	Patchcord,DLC/PC-DLC/PC,Multimode,2mm Parallel,3m	8	11.00	88.00
	MINI-SAS-3	Purchased Cable,MiniSAS Cable,Key246,3m	1	67.00	67.00
	MINI-SAS-6	Outsourcing Cable,External Mini SAS Cable,6.0m,External Mini SAS 26 Pin Plug,24AWG*8P,External Mini SAS 26 Pin Plug	4	91.00	364.00
1.1.1.6	Storage management software				6,074.00
	LIC-S5B-ISM02-BLOCK	HS Integrated Storage Manager-Device Management License for OceanStor Block S5800T	1	4,136.00	4,136.00
	LIC-UltraPath02-V1R5	OceanStor HS UltraPath Software License	1	1,938.00	1,938.00
1.1.1.7	Third Party				6,792.00
	N8GHBA000	QLOGIC QLE2562 HBA Card,PCIE,8Gbps DualPort ,Fiber Channel Multimode LC Optic Interface,English Manual,Driver CD	4	1,698.00	6,792.00
Total of Product					295,522.00
1.1.1.8	Maintenance Support Service				179,568.00
	Hi-Care Premier On-Site Service (3 years)		1	179,568.00	179,568.00

Total of Service (3 years)				179,568.00
Total Price				475,090.00
Notes: Hi-Care Premier On-Site Service include: 7*24 Technical Assistance Center Access. Access to all new software updates and Online Support. 24*7*4 Hours Onsite Hardware Replacement.				